




NEWCLIP
TECHNICS

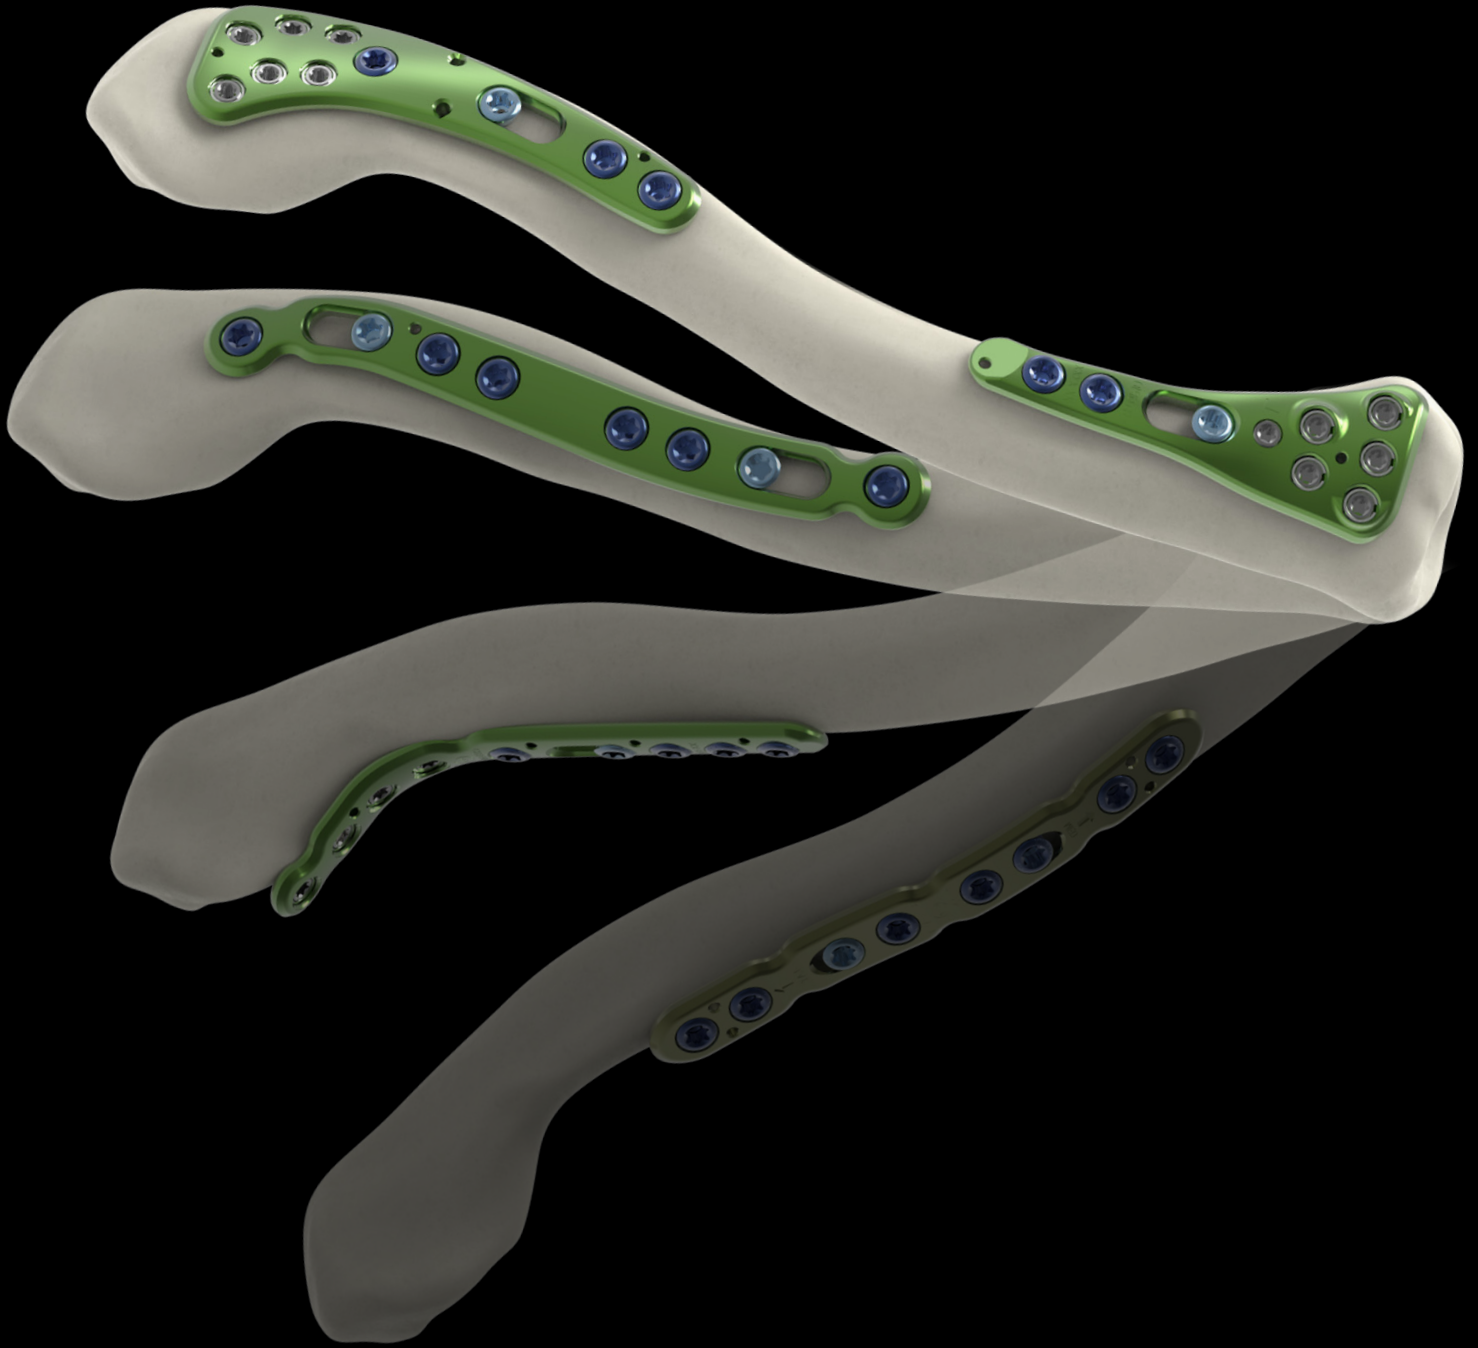

ALIANS
CLAVICLE S

ALIANS CLAVICLE S

Intended purpose: the implants of the Alians Clavicle S range are dedicated to the fixation of fractures, mal-unions, non-unions, and osteotomies of the clavicle in adults.


Contraindications:

- Pregnancy.
- Acute or chronic, local or systemic infections.
- Allergy to one of the materials used or sensitivity to foreign bodies.

A COMPREHENSIVE RANGE OF SUPERIOR PLATES


→ PLATES DEDICATED TO THE LATERAL THIRD OF THE CLAVICLE

I Superior lateral plate

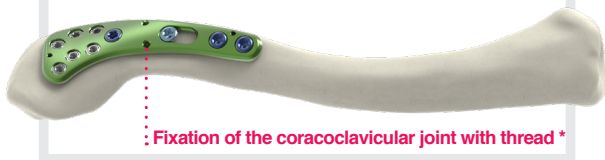

2 sizes available

I Superior lateral bendable plate

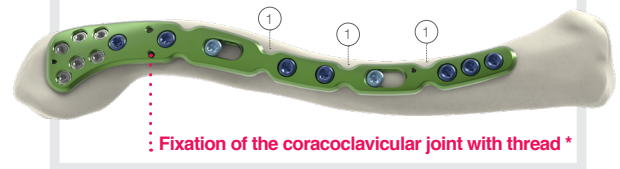

1 size available

I Superior lateral plate with suture holes



1 size available

I Superior extra lateral plate



2 sizes available

① Thanks to their bendable sections, the bendable plates ensure an optimized fit in case of complex fractures and non-unions. The bending irons (ANC452) can be used in these cases (see page 5 for more information).

* The suture holes are compatible with needles $\varnothing 0.9$ mm maximum for the standard lateral plates and $\varnothing 1.2$ mm for the suture plates (CSTxL1D). We recommend using #2 USP (5 Ph. Eur.) and #5 USP (7 Ph. Eur.)

PLATE FEATURES

A COMPREHENSIVE RANGE OF SUPERIOR PLATES


→ PLATES DEDICATED TO THE MIDDLE THIRD OF THE CLAVICLE

I Superior midshaft plate



1 standard size and 2 narrow sizes available

I Superior midshaft bendable plate

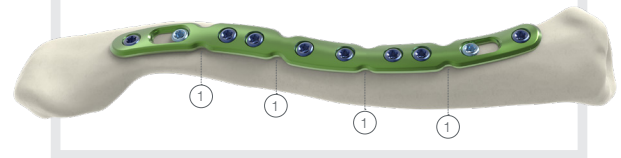


3 sizes available

I Superior lateral midshaft plate



2 sizes available

I Superior lateral midshaft bendable plate

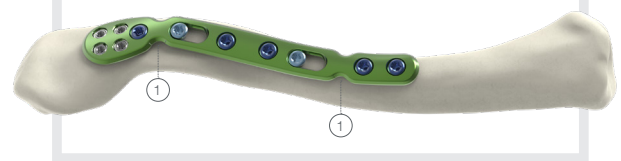

1 size available

① Thanks to their bendable sections, the bendable plates ensure an optimized fit in case of complex fractures and non-unions. The bending irons (ANC452) can be used in these cases (see page 5 for more information).

→ PLATE DEDICATED TO THE MEDIAL THIRD OF THE CLAVICLE

I Superior medial midshaft plate



1 size available

PLATE FEATURES

A COMPREHENSIVE RANGE OF ANTERIOR PLATES

→ PLATE DEDICATED TO THE MIDDLE THIRD OF THE CLAVICLE




1 size available



→ PLATES DEDICATED TO THE LATERAL AND LATERAL MIDSHAFT PART OF THE CLAVICLE



1 size available*

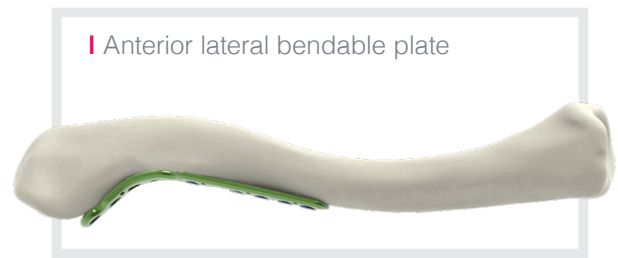

1 size available*

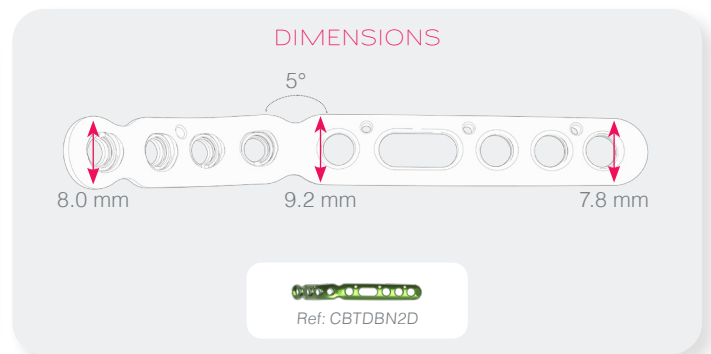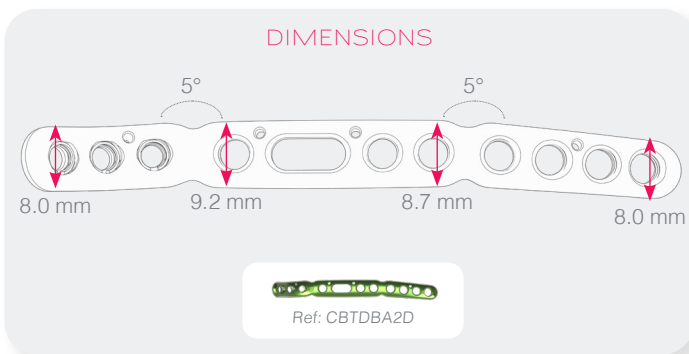

FIXATIONS

- DTS3 polyaxial holes for Ø2.8 mm locking screws (SDT2.8LxD), for lateral and medial plates only.
- Holes for Ø3.5 mm locking (SOT3.5LxD) and non locking screws (CT3.5LxD).
- Oblong holes for Ø3.5 mm non locking screws (CT3.5LxD).

*For anterior lateral plates: full Ø2.8 polyaxial versions are also available. The shape of these plates are strictly identical for both versions.

TECHNICAL FEATURES

PRECONTOURED IMPLANTS

→ OPTIMIZED ANATOMICAL CONGRUENCE


The design of this implant is the result of a proprietary state-of-the-art mapping technology to establish an optimized congruence between the plate and the bone.




→ BENDABLE PLATES

Some plates from the Alians Clavicle S range offer bending areas. It is possible to bend the plate with the bending irons (ANC452) following the instructions below:

- Bending is only possible in the areas intended for this purpose.
- A bendable area should be bent only once and in one direction.
- Bending should not be performed excessively.
- There is a risk of distortion of the holes when bending the plate. Thus, the holes must be protected to avoid damaging the fixation system.

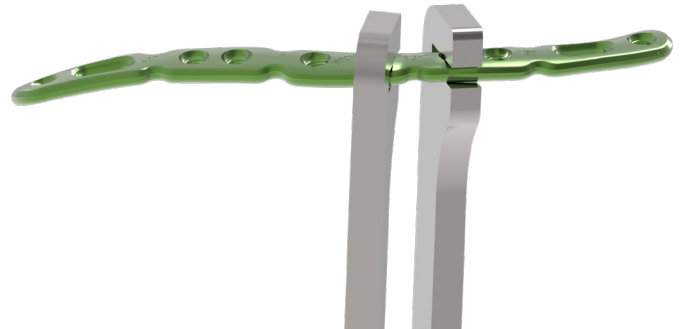

ANGULAR RANGE $\pm 10^\circ$ POLYAXIAL LOCKING FIXATION

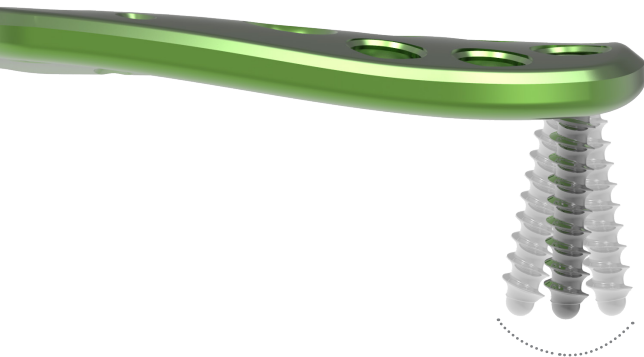

Polyaxiality of 20°


The DTS3 technology ensures the locking of the screw into the plate while allowing its angulation. This system helps for the insertion of the screws in diverging or converging directions and strengthens the assembly.



Dualtec System® III Technology
Polyaxial locking fixation

MONOAXIAL LOCKING SYSTEM

- The screw head is stopped in the hole, ensuring its locking.
- The screw head is buried in the plate.
- Plate and screw made from the same material: titanium alloy.
- Non locking screws (CT3.5LxxD) can be used in the locking holes at the surgeon's discretion.

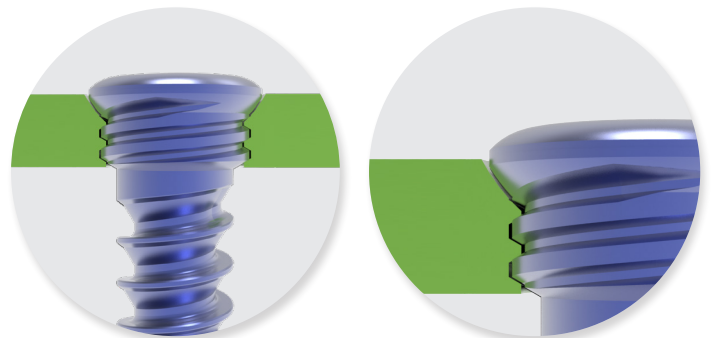


The threads under the screw head and inside the hole have strictly the same characteristics.

TECHNICAL FEATURES

SPECIFIC FIXATIONS FOR THE ANTERIOR MIDSHAFT PLATE SIZE 2


→ LOCKING RAMP OBLONG HOLE

The ramp oblong hole allows a simple and controlled compression **1** by the screw/plate interface or a locked fixation **2** using a locking screw.

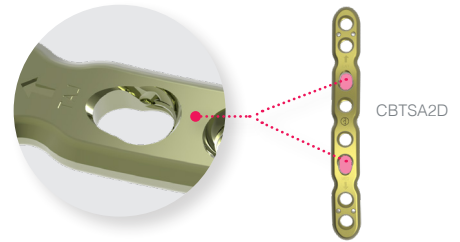


1 DYNAMIC COMPRESSION

⚠ In order to achieve compression, a $\varnothing 3.5$ mm non-locking screw (CT3.5LxxD) can be used. The $\varnothing 2.7$ mm drill bit must be manually maintained to drill in the oval part of the oblong hole located opposite the fracture line. Thus, the insertion of the non locking screw at the top of the ramp allows for the compression of the bone fragments.


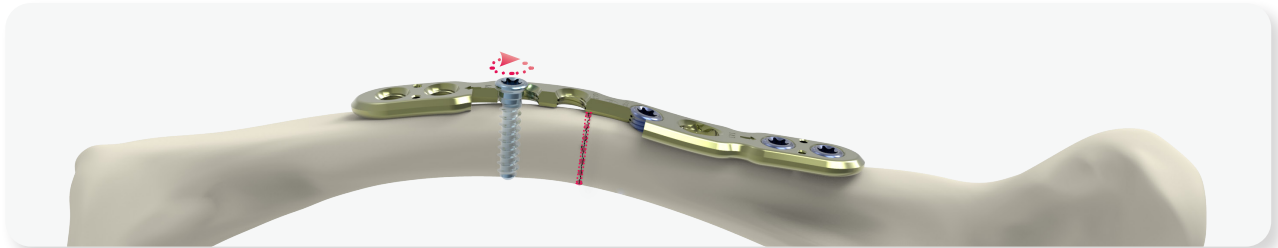


Compression power: 2 mm

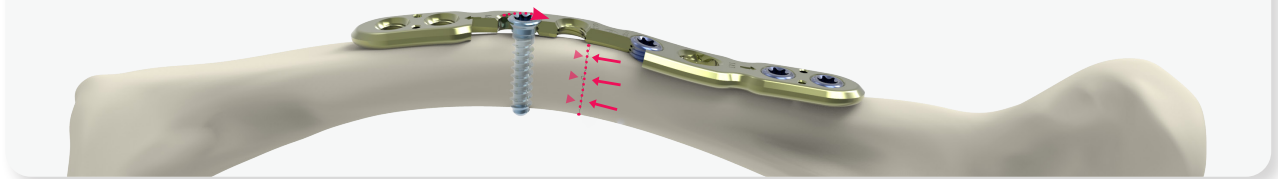

2 LOCKED FIXATION

If no additional compression is required, a $\varnothing 3.5$ mm locking screw (SOT3.5LxxD) can be used. It must be inserted in the locking part of the oblong hole (for the lateral hole in the most medial part and for the medial hole in the most lateral part). To do so, use the $\varnothing 2.7$ mm threaded guide gauge for $\varnothing 3.5$ mm screws (ANC1445).

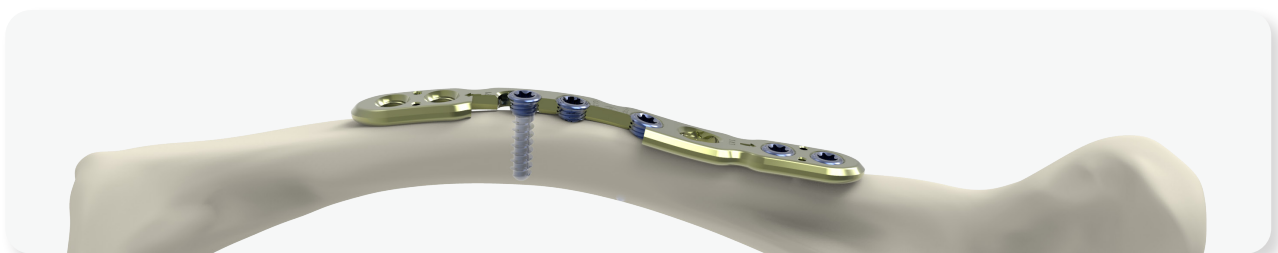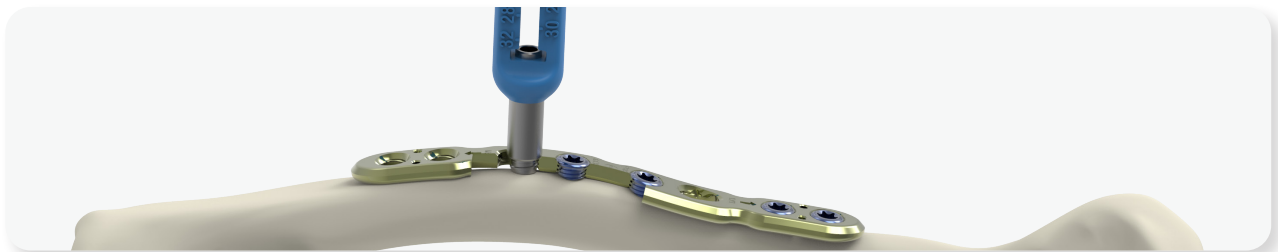

SURGICAL TECHNIQUE

LATERAL MIDSHAFT PLATE

Applicable for all the midshaft plates and lateral midshaft plates with only Ø3.5 mm screws
Example using the size 2 lateral midshaft plate (CTDML2D)

DRILL BITS CHARACTERISTICS


The Alians Clavicle S kit offers two different types of drill bits :

- **Standard drill bits**
 - ANC1356 (Ø2.0 mm)
 - ANC1355 (Ø2.7 mm)
- **Auto-stop drill bits**
 - ANC1357 (Ø2.0 mm)
 - ANC1381 (Ø2.7 mm)

The auto-stop drill bits and the associated guide gauge have been designed for a maximum drilling depth of a 18 mm screw. Therefore, excessive penetration is avoided and surrounding tissues are protected (e.g. subclavian artery).


The choice of using a standard or an auto-stop drill bit is entirely left to the surgeon's discretion. Both versions are fully compatible with the rest of the instrumentation and the only difference is the length of the instrument.

Auto-stop drill bits are identifiable by the laser marked rings on the quick coupling part of the instrument (a).

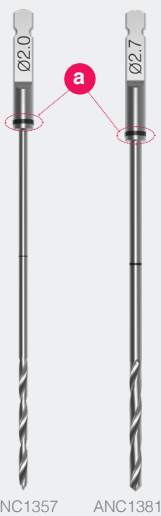


AUTO-STOP DRILL BITS

Ref.	Ø	Max. Length
ANC1357	Ø2.0 mm	18 mm
ANC1381	Ø2.7 mm	18 mm

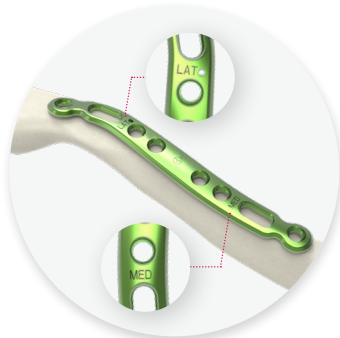


1. The plate can be provisionally fixed on the bone using pliers or using Ø1.2 mm pins (33.0212.120) for the plates with pin holes.

Position the plate using the markings "LAT" (Lateral) and "MED" (Medial).

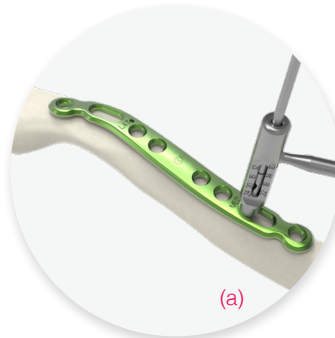

2. Perform the drilling using the non threaded bent guide gauge (ANC1030) and the Ø2.7 mm auto-stop drill bit (ANC1381) in the medial oblong hole.

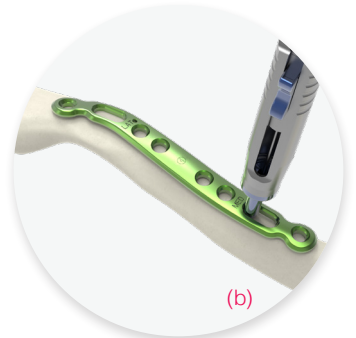


3. Measure the screw length directly on the non-threaded bent guide gauge (ANC1030) (a) or with the length gauge (ANC1028) (b).



4. Insert a non-locking screw (CT3.5LxxD) using the screwdriver (ANC1027).

Repeat the steps 2 to 4 for the remaining oblong hole.

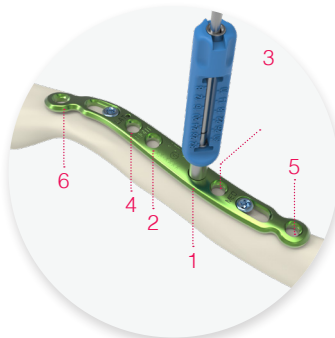

5. Insert the threaded guide gauge (ANC1445) for Ø3.5 mm locking screws (SOT3.5LxxD) starting from the holes located near the fracture to those located at each end of the plate.

Perform drilling using either the Ø2.7 auto-stop drill bit (ANC1381) or the standard drill bit (ANC1355).



6. Measure the screw length directly on the threaded guide gauge (ANC1445) or with the length gauge (ANC1028).

Insert a Ø3.5mm locking screw (SOT3.5LxxD) using the screwdriver (ANC1027).

Repeat steps 5 and 6 for the remaining Ø3.5mm locking screws (SOT3.5LxxD).



FINAL RESULT

SURGICAL TECHNIQUE


LATERAL PLATE

Applicable for all the lateral, midshaft and medial plates with both Ø2.8 mm and Ø3.5 mm screws - example using the size 2 lateral plate (CTDL2D)




1. The plate can be provisionally fixed on the bone using pliers or using Ø1.2 mm pins (33.0212.120) for the plates with pin holes.

Position the plate and perform the drilling using the non-threaded bent guide gauge (ANC1030) and the drill bit (ANC1381 or ANC1355) into the lateral oblong hole.

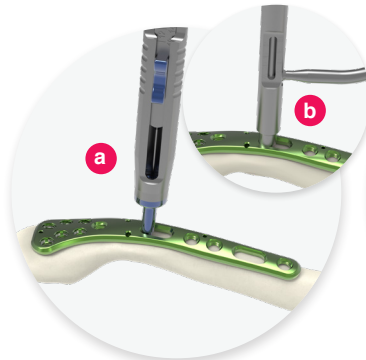


2. Read the screw length using the length gauge (ANC1028) (a) or directly on the non threaded bent guide (ANC1030) (b).

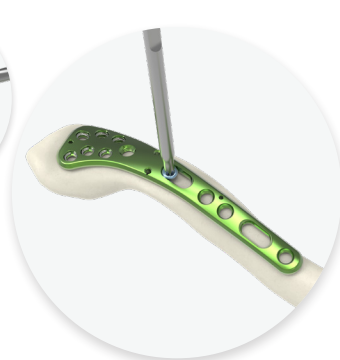

3. Insert a non-locking screw (CT3.5LxxD) using the screwdriver (ANC1027). Repeat the steps 1 to 3 for the remaining oblong hole.



4. Insert the threaded guide gauge (ANC1360) into the epiphyseal part of the plate. Then, angulate as required and perform the drilling using the drill bit (ANC1356).

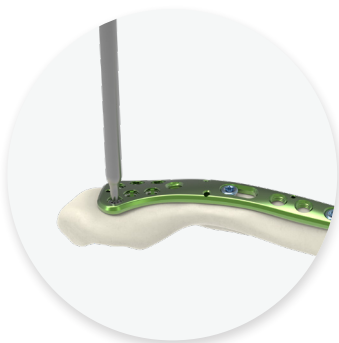

5. Measure the screw length directly on the threaded guide gauge (ANC1360) or with the length gauge (ANC102) .


Insert a Ø2.8 mm locking screw (SDT2.8LxxD) into the plate using the screwdriver (ANC575).

Repeat steps 4 and 5 for the other Ø2.8 mm screws.




6. For the remaining Ø3.5 mm locking screws, insert the threaded guide gauge (ANC1445), perform the drilling (ANC1381 or ANC1355).

We recommend starting from the holes located near the fracture to those located at the end of the plate.

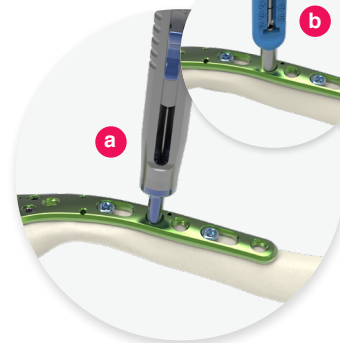

7. Read the screw length using the length gauge (ANC1028) (a), or directly on the threaded guide gauge (ANC1445) (b).

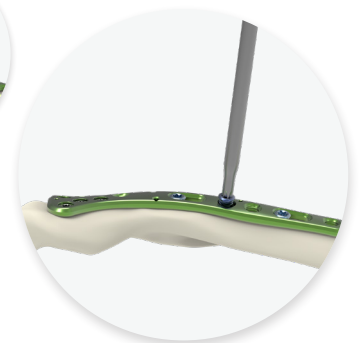

8. Insert a Ø3.5mm locking screw (SOT3.5LxxD) using the screwdriver (ANC1027).

Repeat the same steps for the remaining Ø3.5 mm locking screws (SOT3.5LxxD).






FINAL RESULT

SURGICAL TECHNIQUE

OPTION - DOUBLE GUIDE (AVAILABLE ONLY ON DEMAND)

Surgical technique example for a butterfly fragment surgery with a double guide (ANC1056)

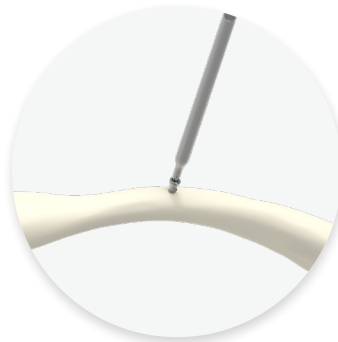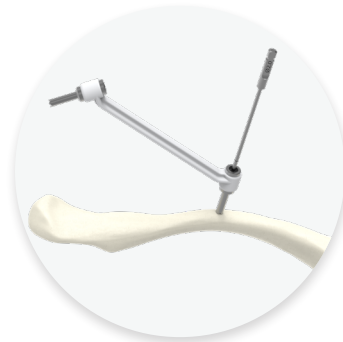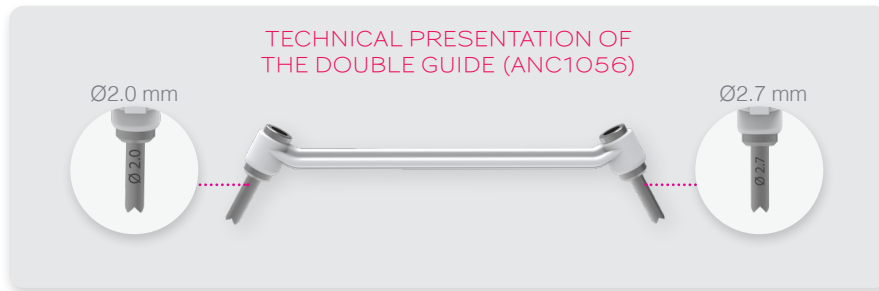

1. Choose correct diameter of the screw (Ø2.8 mm or Ø3.5 mm) for the butterfly fragment.

2. For the Ø2.8 mm screw*, perform the drilling using the correct side of the guide (marked Ø2.0 mm) and with the Ø2.0 mm quick coupling drill bit (ANC1356).

The lag technique can also be performed using the Ø2.7 mm drill bit (ANC1355) on the other side of the guide.

3. Measure the screw length using the length gauge (ANC102).

Insert the Ø2.8 mm screw, using the prehensor screwdriver (ANC575).

FINAL RESULT

* For a Ø3.5 mm screw, use the other side of the guide (marked Ø2.7 mm) with Ø2.7 mm quick coupling drill bit (ANC1355) and the prehensor screwdriver (ANC1027) for the insertion of the screw



IMPLANT REFERENCES

SUPERIOR PLATES

→ EXTRA LATERAL PLATES

SUPERIOR EXTRA LATERAL PLATES

Ref.	Description
CBTDLN1D	Extra lateral clavicle plate - Superior - Right - Size 1 - 8 holes - L44 mm
CBTGLN1D	Extra lateral clavicle plate - Superior - Left - Size 1 - 8 holes - L44 mm
CBTDLN2D	Extra lateral clavicle plate - Superior - Right - Size 2 - 10 holes - L55 mm
CBTGLN2D	Extra lateral clavicle plate - Superior - Left - Size 2 - 10 holes - L55 mm



CBTDLN1D



CBTGLN1D



CBTDLN2D




CBTGLN2D

→ LATERAL PLATES

SUPERIOR LATERAL PLATES

Ref.	Description
CTDL1D	Lateral clavicle plate - Superior - Right - Size 1 - 10 holes - L66 mm
CTGL1D	Lateral clavicle plate - Superior - Left - Size 1 - 10 holes - L66 mm
CTDL2D	Lateral clavicle plate - Superior - Right - Size 2 - 12 holes - L91 mm
CTGL2D	Lateral clavicle plate - Superior - Left - Size 2 - 12 holes - L91 mm



CTDL1D



CTGL1D



CTDL2D



CTGL2D

SUPERIOR LATERAL BENDABLE PLATES

Ref.	Description
CBTDL2D	Lateral bendable clavicle plate - Superior - Right - Size 2 - 15 holes - L138 mm
CBTGL2D	Lateral bendable clavicle plate - Superior - Left - Size 2 - 15 holes - L138 mm



CBTDL2D



CBTGL2D

→ LATERAL SUTURE PLATES

SUPERIOR LATERAL SUTURE PLATES

Ref.	Description
CSTD1D	Lateral clavicle plate - Superior - Right - Size 1 - 11 holes - L68 mm
CSTGL1D	Lateral clavicle plate - Superior - Left - Size 1 - 11 holes - L68 mm



CSTD1D



CSTGL1D

→ LATERAL MIDSHAFT PLATES

SUPERIOR LATERAL MIDSHAFT PLATES

Ref.	Description
CTDML1D	Lateral midshaft clavicle plate - Superior - Right - Size 1 - 6 holes - L79 mm
CTGML1D	Lateral midshaft clavicle plate - Superior - Left - Size 1 - 6 holes - L79 mm
CTDML2D	Lateral midshaft clavicle plate - Superior - Right - Size 2 - 8 holes - L93 mm
CTGML2D	Lateral midshaft clavicle plate - Superior - Left - Size 2 - 8 holes - L93 mm



CTDML1D



CTGML1D



CTDML2D



CTGML2D

SUPERIOR LATERAL MIDSHAFT BENDABLE PLATES

Ref.	Description
CBTDML2D	Lateral midshaft bendable clavicle plate - Superior - Right - Size 2 - 11 holes - L100 mm
CBTGML2D	Lateral midshaft bendable clavicle plate - Superior - Left - Size 2 - 11 holes - L100 mm



CBTDML2D



CBTGML2D

IMPLANT REFERENCES

SUPERIOR PLATES

→ MIDSHAFT PLATES

SUPERIOR MIDSHAFT PLATES - NARROW

Ref.	Description
CTDMN1D	Midshaft clavicle plate - Superior - Narrow - Right - Size 1 - 6 holes - L73 mm
CTGMN1D	Midshaft clavicle plate - Superior - Narrow - Left - Size 1 - 6 holes - L73 mm
CTDMN2D	Midshaft clavicle plate - Superior - Narrow - Right - Size 2 - 6 holes - L91 mm
CTGMN2D	Midshaft clavicle plate - Superior - Narrow - Left - Size 2 - 6 holes - L91 mm




SUPERIOR MIDSHAFT PLATES

Ref.	Description
CTDM2D	Midshaft clavicle plate - Superior - Right - Size 2 - 8 holes - L89 mm
CTGM2D	Midshaft clavicle plate - Superior - Left - Size 2 - 8 holes - L89 mm



SUPERIOR MIDSHAFT BENDABLE PLATES

Ref.	Description
CBTDM1D	Midshaft bendable clavicle plate - Superior - Right - Size 1 - Right - 6 holes - L83 mm
CBTGM1D	Midshaft bendable clavicle plate - Superior - Left - Size 1 - Left - 6 holes - L83 mm
CBTDM1.5D	Midshaft bendable clavicle plate - Superior - Right - Size 1.5 - 10 holes - L105 mm
CBTGM1.5D	Midshaft bendable clavicle plate - Superior - Left - Size 1.5 - 10 holes - L105 mm
CBTDM2D	Midshaft bendable clavicle plate - Superior - Right - Size 2 - 10 holes - L127 mm
CBTGM2D	Midshaft bendable clavicle plate - Superior - Left - Size 2 - 10 holes - L127 mm

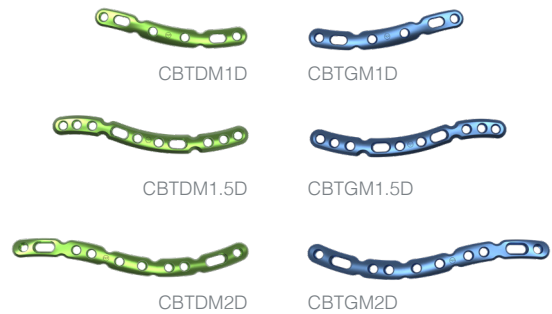

→ MEDIAL MIDSHAFT PLATES

SUPERIOR MEDIAL MIDSHAFT PLATES

Ref.	Description
CBTDP1D	Medial midshaft clavicle plate - Superior - Right - Size 1 - 9 holes - L56 mm
CBTGP1D	Medial midshaft clavicle plate - Superior - Left - Size 1 - 9 holes - L56 mm



IMPLANT REFERENCES

ANTERIOR PLATES

→ MIDSHAFT PLATES

ANTERIOR MIDSHAFT BENDABLE PLATE

Ref.	Description
CBTSA2D	Midshaft bendable clavicle plate - Anterior - Symmetrical - Size 2 - 8 holes - L77 mm



CBTSA2D

→ LATERAL MIDSHAFT PLATES

ANTERIOR LATERAL MIDSHAFT BENDABLES PLATES

Ref.	Description
CBTDBA2D	Lateral midshaft bendable clavicle plate - Anterior - Right - Size 2 - 11 holes - L89 mm
CBTGBA2D	Lateral midshaft bendable clavicle plate - Anterior - Left - Size 2 - 11 holes - L89 mm
CBTDBA2D2.8*	Lateral midshaft bendable polyaxial clavicle plate - Anterior - Right - Size 2 - 11 holes - L89 mm
CBTGBA2D2.8*	Lateral midshaft bendable polyaxial clavicle plate - Anterior - Left - Size 2 - 11 holes - L89 mm



CBTDBA2D

(CBTDBA2D2.8*)



CBTGBA2D

(CBTGBA2D2.8*)

→ LATERAL PLATES

ANTERIOR LATERAL BENDABLES PLATES

Ref.	Description
CBTDBN2D	Lateral bendable clavicle plate - Anterior - Right - Size 2 - 9 holes - L71 mm
CBTGBN2D	Lateral bendable clavicle plate - Anterior - Left - Size 2 - 9 holes - L71 mm
CBTDBN2D2.8*	Lateral bendable polyaxial clavicle plate - Anterior - Right - Size 2 - 9 holes - L71 mm
CBTGBN2D2.8*	Lateral bendable polyaxial clavicle plate - Anterior - Left - Size 2 - 9 holes - L71 mm



CBTDBN2D
(CBTDBN2D2.8*)




CBTGBN2D
(CBTGBN2D2.8*)

* Anterior lateral and lateral midshaft plates also available in Ø2.8 polyaxial versions. Only the screw platform is different, the rest of the design remains strictly identical - option available only on demand

SCREW REFERENCES


→ Ø3.5 MM SCREWS



LOCKING SCREWS*

Ref.	Description
SOT3.5L10D	Ø3.5 mm locking screw - L10 mm
SOT3.5L12D	Ø3.5 mm locking screw - L12 mm
SOT3.5L14D	Ø3.5 mm locking screw - L14 mm
SOT3.5L16D	Ø3.5 mm locking screw - L16 mm
SOT3.5L18D	Ø3.5 mm locking screw - L18 mm
SOT3.5L20D	Ø3.5 mm locking screw - L20 mm
SOT3.5L22D	Ø3.5 mm locking screw - L22 mm
SOT3.5L24D	Ø3.5 mm locking screw - L24 mm

* Blue anodized




NON-LOCKING SCREWS*

Ref.	Description
CT3.5L10D	Ø3.5 mm Non-locking screw - L10 mm
CT3.5L12D	Ø3.5 mm Non-locking screw - L12 mm
CT3.5L14D	Ø3.5 mm Non-locking screw - L14 mm
CT3.5L16D	Ø3.5 mm Non-locking screw - L16 mm
CT3.5L18D	Ø3.5 mm Non-locking screw - L18 mm
CT3.5L20D	Ø3.5 mm Non-locking screw - L20 mm
CT3.5L22D	Ø3.5 mm Non-locking screw - L22 mm
CT3.5L24D	Ø3.5 mm Non-locking screw - L24 mm

* Light blue anodized


→ Ø2.8 MM SCREWS



LOCKING SCREWS*

Ref.	Description
SDT2.8L10D	Ø2.8 mm locking screw - L10 mm
SDT2.8L12D	Ø2.8 mm locking screw - L12 mm
SDT2.8L14D	Ø2.8 mm locking screw - L14 mm
SDT2.8L16D	Ø2.8 mm locking screw - L16 mm
SDT2.8L18D	Ø2.8 mm locking screw - L18 mm
SDT2.8L20D	Ø2.8 mm locking screw - L20 mm
SDT2.8L22D	Ø2.8 mm locking screw - L22 mm
SDT2.8L24D	Ø2.8 mm locking screw - L24 mm
SDT2.8L26D	Ø2.8 mm locking screw - L26 mm
SDT2.8L28D	Ø2.8 mm locking screw - L28 mm
SDT2.8L30D	Ø2.8 mm locking screw - L30 mm
SDT2.8L32D	Ø2.8 mm locking screw - L32 mm

* Not anodized



NON-LOCKING SCREWS*

Ref.	Description
CT2.8L10D	Ø2.8 mm Non-locking screw - L10 mm
CT2.8L12D	Ø2.8 mm Non-locking screw - L12 mm
CT2.8L14D	Ø2.8 mm Non-locking screw - L14 mm
CT2.8L16D	Ø2.8 mm Non-locking screw - L16 mm
CT2.8L18D	Ø2.8 mm Non-locking screw - L18 mm
CT2.8L20D	Ø2.8 mm Non-locking screw - L20 mm
CT2.8L22D	Ø2.8 mm Non-locking screw - L22 mm
CT2.8L24D	Ø2.8 mm Non-locking screw - L24 mm


* Pink anodized

REMARK

All the implants are also available in a sterile version. An «-ST» is added to the end of the reference.

Ex : «SDT2.8L10D-ST»


→ OPTIONAL SCREWS (AVAILABLE ONLY ON DEMAND)



Ø2.8 MM NON LOCKING POLYAXIAL SCREWS*

Ref.	Description
QDT2.8LxxD	Ø2.8 mm non-locking screw - L10 to 32 mm (2 mm incrementation)


* Yellow anodized



Ø2.8 MM NON LOCKING SCREWS FOR Ø3.5MM HOLES*

Ref.	Description
CET2.8LxxD	Ø2.8 mm non-locking screw - Oblong 3.5 - L10 to 24 mm (2 mm incrementation)

* Brown anodized



Ø2.8 MM LOCKING SCREWS FOR Ø3.5MM HOLES*

Ref.	Description
SOT2.8LxxD	Ø2.8 mm locking screw - Oneclip 3.5 - L10 to 24 mm (2 mm incrementation)

* Turquoise anodized

Remark: please note that the «xx» in the references represent the length of the screw.
Ex: the reference for the Ø2.8 mm non locking screw - L10 mm is «QDT2.8L10D».

INSTRUMENT REFERENCES

INSTRUMENTS		
Ref.	Description	Qty
ANC102	Length gauge for Ø2.8 mm screws	1
ANC195	Clamp 14 cm with ball Ø5 mm	2
ANC251	18 cm verbrugge forceps	2
ANC350	Ø4.5 mm AO quick coupling handle - Size 1	1
ANC351	Ø4.5 mm AO quick coupling handle - Size 2	1
ANC452	Bending iron	2
ANC575	T8 quick coupling screwdriver	2
ANC986	Ø2.0 mm non threaded bent guide gauge for Ø2.8 mm screws	1
ANC1027	T15 AO quick coupling prehensor screwdriver	2
ANC1028	Length gauge for Ø3.5 mm screws	1
ANC1030	Ø2.7 mm non threaded bent guide gauge for Ø3.5 mm screws	1
ANC1056*	Double guide Ø2.8 mm / Ø2.1 mm for Ø2.8 mm screws	1
ANC1355	Ø2.7 mm quick coupling drill bit - L125 mm	1
ANC1356	Ø2.0 mm quick coupling drill bit - L125 mm	1
ANC1357	Ø2.0 mm quick coupling drill bit for 18 mm screws	1
ANC1360	Ø2.0 mm threaded guide gauge for Ø2.8 mm screws	2
ANC1381	Ø2.7 mm quick coupling drill bit for 18 mm screws	1
ANC1445	Ø2.7 mm threaded guide gauge for Ø3.5 mm screws	2
33.0212.120	Pin Ø1.2 L120 mm	8

* Optional instrument, available only on demand


REMOVAL KIT

If you have to remove ALIANS CLAVICLE S implants, make sure to order the Newclip Technics removal set, which includes the following instrument:






- ANC350: Ø4.5 mm AO quick coupling handle - Size 1
- ANC351: Ø4.5 mm AO quick coupling handle - Size 2
- ANC575: T8 quick coupling screwdriver - for Ø2.8 mm screws
- ANC974: T15 quick screwdriver - for Ø3.5 mm screws

KIT DESCRIPTION

→ TOP LEVEL

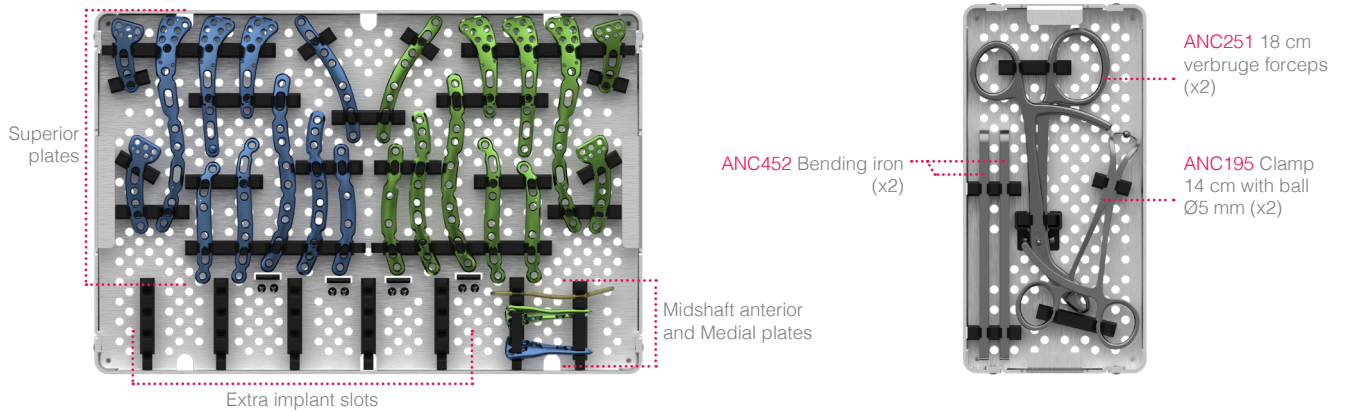

→ LOWER LEVEL

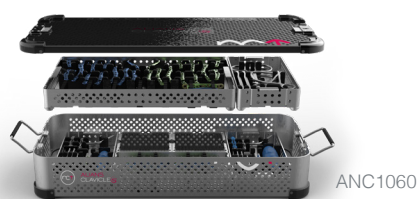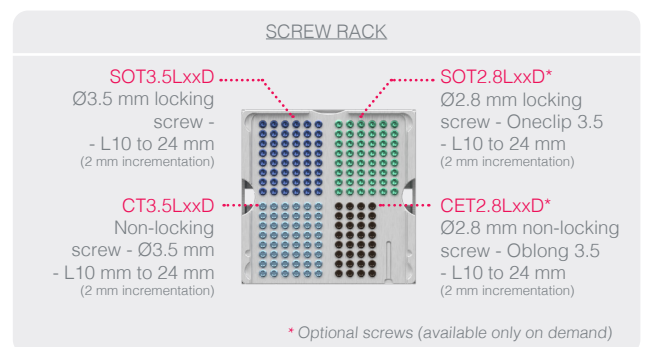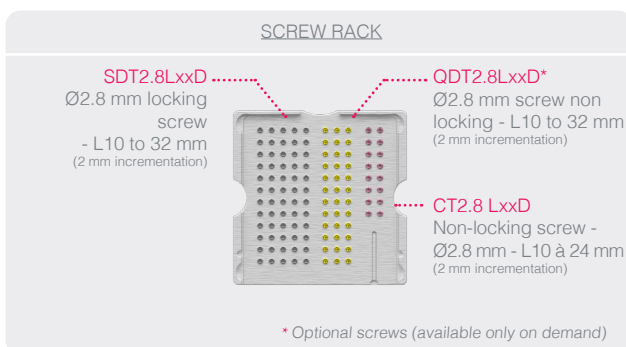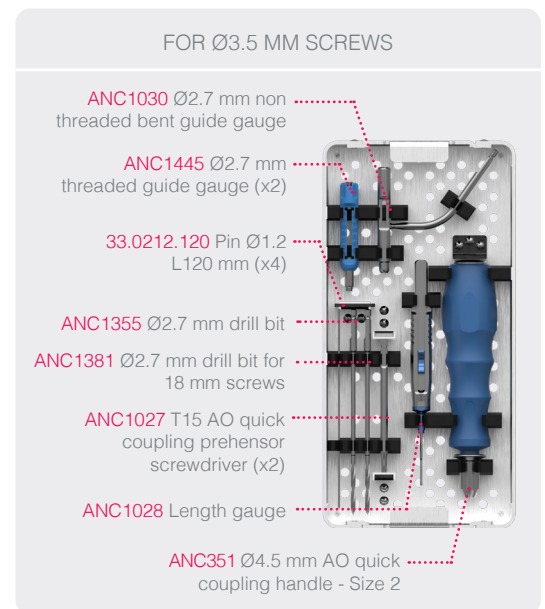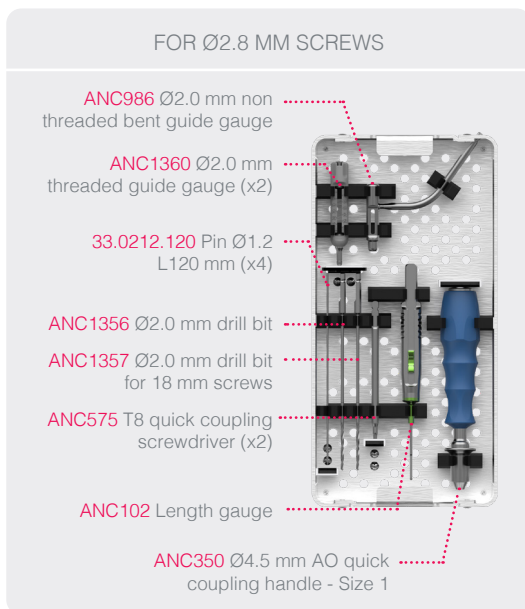

This information is intended to demonstrate the Newclip Technics portfolio of medical devices. Always refer to the package insert, product label and/or user instructions including cleaning and sterilization before using any Newclip Technics product. These products must be handled and/or implanted by trained and qualified staff who have read the instructions before use. A surgeon must always rely on her or his own professional clinical judgement when deciding whether to use a particular product when treating a particular patient. Product availability is subject to the regulatory or medical practices that govern individual markets. Please contact your Newclip Technics representative if you have questions about the availability of Newclip Technics products in your area.

NEWCLIP TECHNICS

45 rue des Garottières
44115 Haute Goulaine, France
+33 (0)2 28 21 23 25
orders@newcliptechnics.com
www.newcliptechnics.com

NEWCLIP TECHNICS GERMANY

Newclip GmbH
Pröllstraße 11
D-86157 Augsburg, Germany
+49 (0)821 650 749 40
info@newclipgmbh.com
www.newclipgmbh.de

NEWCLIP TECHNICS USA

Newclip USA
340 Tesconi Circle,
Santa Rosa CA 95403, USA
+1 707 230 5078
customerservice@newclipusa.com
www.newclipusa.com

NEWCLIP TECHNICS AUSTRALIA

Newclip Australia
3B/11 Donkin Street
West End 4101, Australia
+61 (0)2 81 886 110
solutions@newclipaustralia.com
www.newcliptechnics.com

NEWCLIP TECHNICS JAPAN

Newclip Technics Japan K.K.
KKK Bldg. 502, 3-18-1 Asakusabashi
Taito-Ku, Tokyo, 111-0053, Japan
+81 (0)3 58 25 49 81
Fax: +81 (0)3 58 25 49 86
www.newcliptechnics.com

NEWCLIP TECHNICS IBERIA

Newclip Iberia
Calle Frederic Mompou, 4b
Sant Just Desvern, 08960 Barcelona, Spain
+34 938 299 526
contact@newclipiberia.com
www.newcliptechnics.com