

Medtronic

MiniMed™ Mobile app

Quick Reference Guide

Getting started

1 Get started



Check your local Medtronic website to make sure your mobile device is compatible with the MiniMed™ Mobile app.



Download and install the MiniMed™ Mobile app from the Google Play™ or Apple App Store®.

WiFi or mobile data connection is needed for set-up.


2 Begin setup

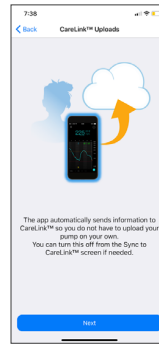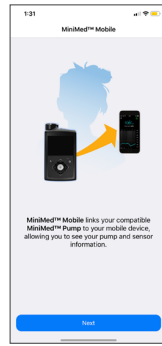

View information screens about the app.


Note: Care partners can use the CareLink™ Connect app.

3 CareLink™ account

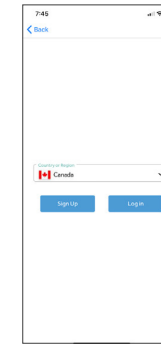


Log in if you already have a CareLink™ account. If not, tap **Sign Up**. Proceed until logged in.

4 Pair your pump to the MiniMed™ Mobile app

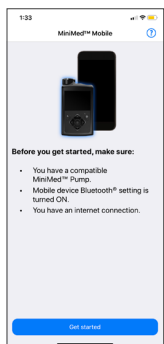


Be sure all three statements are true.

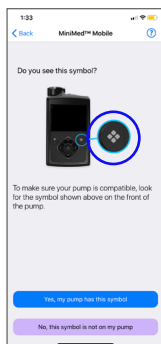


If you do not see this symbol, you cannot use this app. If there is a symbol, continue.


Check for this symbol.

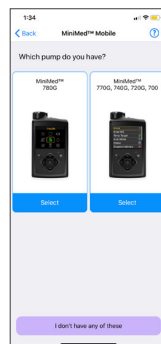


Select the pump that you have. **Note:** If asked, you must allow notifications and make data available.

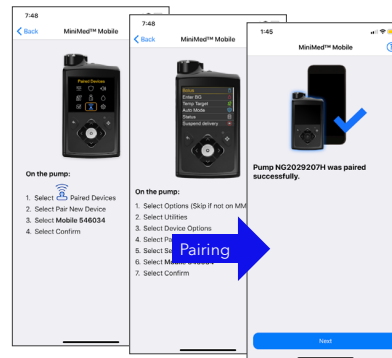

Follow the steps provided to start pairing on the pump. **Note:** If asked, tap **Pair** on the app.

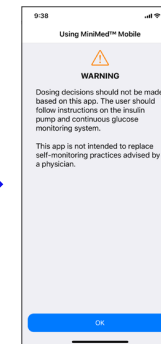

Read and agree to the warning information.

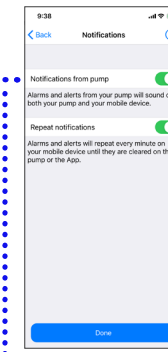

Turn on to receive notifications on both pump and app. If turned on, notifications repeat every minute until dismissed on app.


Home screen



Tap icon for information


Tap icon for event details

Pinch or stretch the graph to change the amount of time displayed.

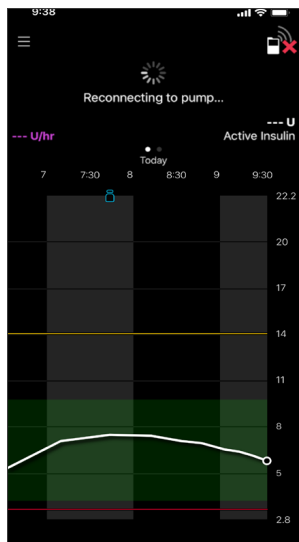


Reconnecting to Pump... appears when the pump and app have been out of range. Allow 60 seconds to reconnect.

Time in range

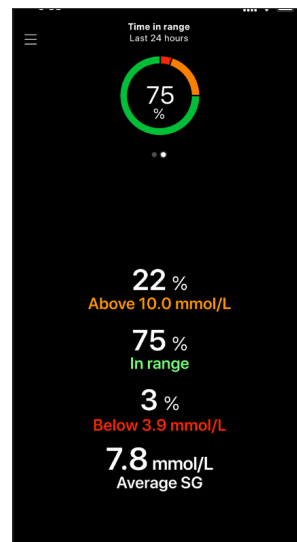

Swipe left on the upper area of the Home screen.

Tap for menu

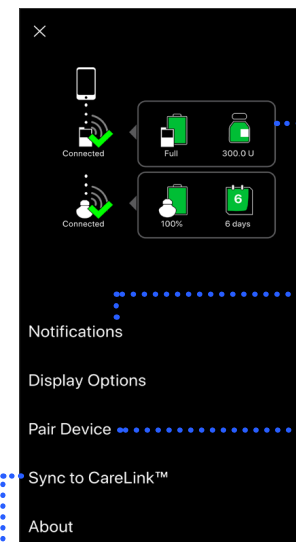


Status: see the status of pump and CGM devices

Notifications: use to change settings

Pair Device: use if pump and app need need to be re-paired

Sync to CareLink™: Use **Upload Now** to upload current data for reports. Use **Manage Care Partners** to approve or remove care partners.

Notifications

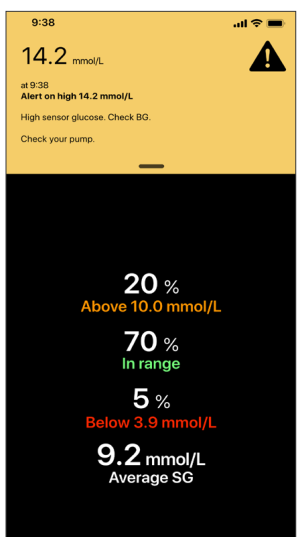

Alarms appear in red

Alerts appear in yellow

Reminders appear in grey

Messages appear in blue




Notifications are not being received on app if this appears at the top of the Home screen.

Tap to turn **Notifications** on.

Note: These must be cleared on the pump even if they are dismissed on the app.

Important:

- If a care partner requests to follow you, go to the menu, to **Sync to CareLink** and to **Manage Care Partners** to accept the request.
- For information to be sent to the CareLink™ Connect app, the MiniMed Mobile app must be:
 - within 6 meters (20 feet of the pump)
 - have internet connection
 - be logged into CareLink™ Personal on the app
 - have **Sync to CareLink™** turned on
- If you have questions, tap  and go to **About**. You will find information on many topics there.