

# Light Absorptance of Algal Films for Photosynthetic Rate Determinations

Raymond J. RITCHIE (✉ [Raymond.Ritchie@alumni.sydney.edu.au](mailto:Raymond.Ritchie@alumni.sydney.edu.au))

Prince of Songkla University in Phuket

Suhailar SMA-AIR

Prince of Songkla University in Phuket

John W. RUNCIE

University of Sydney

---

## Method Article

**Keywords:** Absorptance, Algal films, Algal mats, Electron Transport Rate, Absorptance Factor, PAM fluorometry

**Posted Date:** April 20th, 2022

**DOI:** <https://doi.org/10.21203/rs.3.rs-1556898/v1>

**License:**   This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

---

# Abstract

A Reflectance Absorptance Transmittance (RAT) meter, developed for routine measurements of  $Abt_{\lambda \text{ nm}}$  on leaves, was used to measure absorptance of algal films mounted on glass fibre filter disks for use in PAM (Pulse Amplitude Modulation) fluorometry. Absorptance readings ( $Abt_{\lambda \text{ nm}}$ ) are essential to quantitate the photosynthetic electron transport rate from PAM data and are also helpful if algal disks are used in an IRGA (InfraRed Gas Analyzer). Measurements were made on *Synechococcus R-2* (Cyanophyceae), *Acaryochloris marina* (Chlorobacteria), *Chlorella vulgaris* (Chlorophyceae), *Chaetoceros sp.* (Bacillariophyceae) and *Isochrysis sp.* (Haptophyta) in blue (445 nm), green (525 nm) and red (625 nm) light. Plots of  $Abt_{\lambda}$  vs. Chl *a* ( $\text{mg Chl } a \text{ m}^{-2}$ ) or Chl *d* for *Acaryochloris* ( $\text{mg Chl } d \text{ m}^{-2}$ ) of the algae followed exponential saturation curves ( $Abt_{\lambda} = Abt_{\lambda, \infty} (1 - e^{-k \times \text{Chl}})$ ) usually reaching asymptotes in the blue light used by blue-diode PAM machines. *Synechococcus*, *Chlorella*, *Chaetoceros* and *Isochrysis*  $Abt_{\%445\text{nm}}$  saturates  $\approx 50\text{--}100 \text{ mg Chl } a \text{ m}^{-2}$  (*Synechococcus*:  $Abt_{\%445 \text{ nm}, \text{max}} = 77.3 \pm 0.94, \pm 95\% \text{ conf. limits}$ , *Chlorella*:  $Abt_{\%445 \text{ nm}, \text{max}} = 77.0 \pm 2.06$ , *Chaetoceros*:  $Abt_{\%445 \text{ nm}, \text{max}} = 80.6 \pm 1.87$ ; *Isochrysis*:  $83.2 \pm 8.06 \text{ mg Chl } a \text{ m}^{-2}$ ); *Acaryochloris* above about  $100 \text{ mg Chl } d \text{ m}^{-2}$ . Asymptotic loading of cells was in general easily achieved in blue light in the case of *Synechococcus*, *Chlorella* and *Acaryochloris* but not in green, red or “white” light. It was difficult to achieve asymptotic loading for *Chaetoceros* and *Isochrysis* due to mucilaginous blockage of the filter disks.

## Introduction

We describe the application of a Reflectance-Absorptance-Transmittance (RAT) meter designed by Aquation Pty Ltd, Australia to experimentally measure the absorptance of unicellular algae and photosynthetic bacteria mounted onto glass fibre disks (Ritchie and Runcie 2013, 2014). The RAT meter uses a Red-Green-Blue (RGB) diode as a light source to provide blue (445 nm), green (525 nm) or red (625 nm) light sources similar to those wavelengths used by blue and red-diode based Pulse Amplitude Modulation (PAM) machines. We show that the RAT meter provides a convenient method for estimating absorptance in the laboratory and field for algal and photosynthetic bacterial films compared with Taylor-absorption sphere based methods. The non-destructive method enables measurement of films of photosynthetic organisms on a glass fibre disc if the same algal disk is used for PAM measurements. Glass fibre disks impregnated with algae are also a convenient method of estimating algal respiration and photosynthesis using IRGA (InfraRed Gas Analysers) where the absorptance of the experimental material is also an important consideration.

Modulated fluorescence-based techniques such as those used by PAM machines and Photosynthetic Efficiency Apparatus (PEA) are very useful for estimating photosynthetic electron transport rate (ETR). They offer the great advantage of speed of measurement and hence very large amounts of data can be collected in short periods of time. PAM and PEA methods make particular demands on adequate measurements of irradiance because not only is electromagnetic radiation a required input for ETR calculations but photosynthesis is also calculated from variable fluorescence light output. Photosynthetic

rate as ETR is calculated from the product of the fluorescence-based calculation of the quantum yield of photochemical energy conversion (Genty et al. 1989; Krause and Weis 1991; Schreiber et al. 1995; Figueroa et al. 2003), a photosystem II/I allocation factor (for oxygenic photosynthetic organisms the (assumed) allocation factor is 0.5; Melis 1989), the incident irradiance (E) and the (photosynthetic) absorptance ( $Abt_{\lambda \text{ nm}}$ ) of the incident light (Ritchie and Runcie 2014). Hence, knowing the amount of light absorbed by the photo organism (Absorptance,  $Abt_{\lambda \text{ nm}}$ ) is essential to calculate the photosynthetic rate using PEA or PAM machines. Absorptance values are also essential for calculations of photosynthetic efficiency where photosynthesis is measured using oxygen,  $^{14}\text{CO}_2$  or  $\text{CO}_2$  monitoring methods. Some photosynthetic organisms have non-photosynthetic absorbing pigments: these may sometimes need to be taken into account, particularly for “white” light absorptance determinations in apparatus using a “white” light source.

Absorptance ( $Abt_{\lambda \text{ nm}}$ ) is defined as the amount of irradiance absorbed by a translucent object and is usually expressed as a percentage ( $Abt\%_{\lambda \text{ nm}}$ ) with the wavelength or spectral range of the light source specified. Absorptance is calculated as  $Abt\%_{\lambda \text{ nm}} = 100 - T\%_{\lambda \text{ nm}} - R\%_{\lambda \text{ nm}}$  where,  $T\%_{\lambda \text{ nm}}$  is the percentage transmittance through the object at a given wavelength and  $R\%_{\lambda \text{ nm}}$  is the percentage reflected irradiance.

Many PAM studies use a standard default absorptance value ( $Abt_F$ ) of 0.84 (or  $Abt\%_F = 84$ ) derived from a study using a Taylor Sphere by Björkman and Demmig (1987) for PPFD (400–700 nm) irradiance. It is the default value often incorporated into the software of popular PAM machines. Estimates of ETR based on  $Abt_F = 0.84$  are most properly designated relative ETR (rETR) to reflect the fact that they are based on an experimentally measured fluorescence yield ( $Y$  or  $\Phi_{\text{PSII}}$ ) (Genty et al. 1989; Schreiber et al. 1995) and PPFD (400–700 nm) irradiance ( $\text{mol photon m}^{-2} \text{ s}^{-1}$ ) but not on an experimentally determined absorptance value ( $Abt\%_{\lambda \text{ nm}}$ ).

When using a PAM machine, the default absorptance value of 0.84 ( $Abt_F$  or  $Abt_{400-700 \text{ nm}} \approx 0.84$ ) is not appropriate for unicellular algal films when using a blue or red diode light source (Ritchie and Runcie 2014) nor for photosynthetic bacteria using a blue-light source (Ritchie and Runcie 2013). The standard absorptance value ( $Abt_F$ ) is derived from measurements of absorptance of leaves, not algal films, and the value from Björkman and Demmig (1987) is an overall mean calculated for the whole PPFD range (400–700 nm) not blue or red light sources. Calculation of ETR from data obtained using a blue-diode PAM requires absorptance values for blue light ( $Abt\%_{445\text{nm}}$ ) and a red-diode based PAM machine requires absorptance values for red light. For a PAM machine using a “white” actinic light source (solar temperature  $\approx 5778 \text{ K}$ ) absorptance values for “white” light ( $PPFD_{400-700 \text{ nm}}$ ) are needed. An estimate of  $Abt\%_{400-700 \text{ nm}}$  requires either absorptance measurements under blue, green and red light or using a “white” light source such as an RGB diode with currents applied to the red, green and blue channels to provide an approximate “white” light (Ritchie and Runcie 2014). Some studies have used a Taylor sphere fitted with a quartz halogen 6000 K light source to estimate  $Abt\%_{400-700 \text{ nm}}$  for macroalgae and aquatic

macrophytes (Frost-Christensen and Sand-Jensen 1992; Mercado et al. 1996; Cebrian et al. 1999; Longstaff et al. 2002; Figueroa et al. 2003; Runcie and Durako 2004) or other setups (Figueroa et al. 2009). Schultz (1996) used natural sunlight as the light source for his Taylor sphere. Absorptance measurements are needed for attempts to calculate quantum efficiency of photosynthesis (Ritchie 2010).

Average absorptance values of about 0.95 for 445 nm (blue) and about 0.89 for red light sources (625 nm) are found in a range of mature leaves of vascular plants (Ritchie and Runcie 2014). Some seagrasses have absorptance properties very like terrestrial vascular plant leaves (*Posidonia*, Runcie and Durako 2004) but Ritchie and Runcie (2014) point out that in the case of some xerophytes, seagrasses such as *Halophila* and freshwater aquatic angiosperms absorptances may range to as low as 0.30 for mature leaves. The low absorptances of some seagrasses are attributed to their photosynthetic epidermal cells and lack of palisade mesophyll. This explanation would also account for the low absorptances generally found in the few macrophytic algae where absorptances have been measured (several species, Frost-Christensen and Sand-Jensen 1992; Mercado et al. 1996; Figueroa et al. 2009; epiphytes on the seagrass *Posidonia oceanica*, Cebrian et al. 1999; *Ulva*, Longstaff et al. 2002; *Ulva* and *Porphyra*, Figueroa et al. 2003; *Ulva*, Beach et al. 2006). Absorptances of macroalgae vary enormously even for the same species or genus, for example Beach et al. (2006) noted that despite *Ulva* species being algae with very favourable flat sheet morphology for absorptance studies, various researchers have found absorptances ranging from 19 to 93%. To complicate matters, Figueroa et al. (2009) noted strong seasonal variation in *Ulva*. Such absorptance ranges would change the calculated ETR by a factor of nearly 5, depending on which absorptance factor was used in calculating ETR. Attempts to correlate photosynthetic ETR with photosynthetic measurements using other methods such as  $^{14}\text{C}$  or oxygen electrodes often do not tally very well. Some of this may be due to situations where absorptances were not measured experimentally (e.g. studies on *Ulva*, Beer et al. 2000; Longstaff et al. 2002; Carr and Björk 2003; Beach et al. 2006) compared to studies where absorptances of *Ulva* were measured (Figueroa et al. 2009).

The usual method for measuring the amount of light absorbed by a plant is to use a Taylor or Ulbricht Integrating sphere attached to a spectroradiometer or spectrophotometer. Integrating sphere methods have previously been limited by the prohibitive costs and the cumbersome nature of the experimental setup, particularly for field work (Runcie and Durako 2004; Ritchie and Runcie 2014) but spectrophotometers with Integrating Spheres (Taylor Sphere attachments) are now more readily available (Ritchie and Sma-Air 2020a, b). Little information is available on absorptances of non-vascular terrestrial plants and other photosynthetic organisms such as algal films of *Chlorella*, *Trebouxia*, *Trentepohlia* or *Chlorococcum* mounted on glass fibre disks: Ritchie and Runcie 2013; Ritchie 2014; Chandaravithoon et al. 2018, 2020; Ritchie and Heembo 2021 Ritchie and Sma-Air 2022, macrophytic algae (Frost-Christensen and Sand-Jensen 1992; Mercado et al. 1996; Cebrian et al 1999; Longstaff et al. 2002; Figueroa et al. 2003; Figueroa et al. 2009), lichens (Solhaug et al. 2010; Ritchie 2014), corals etc.: Beer et al. 1998, 2000; Enríquez et al. 2005; Stambler and Dubinsky 2005; Rodríguez-Román et al. 2006; Hennige

et al. 2009). Most PAM-based estimates of ETR on such organisms are actually rETR measurements because experimentally determined absorptances were unavailable.

The present study focuses on the absorptances of algal-impregnated filter disks. However, the absorptance characteristics of photosynthetic mats or surfaces are of great interest physiologically, ecologically and from an evolutionary point of view for example microbial mats, encrusting algae, corals, stromatolites and cushions of bryophytes (Larkum et al. 2018; Hennige et al. 2009; Ritchie 2013, 2014; Ritchie and Heembo 2021; Ritchie and Sma-Air 2022). Algal mats also have biotechnological potential where it may be important to know how much light is actually absorbed.

## Materials And Methods

### *Culturing the Cells:*

The cyanobacterium *Synechococcus* PCC7942 was originally obtained from the Pasteur Culture Collection (PCC). *Acaryochloris marina* (MBIC11017) (Miyashita & Chihara) was a gift from A.W.D. Larkum (UTS-Sydney, NSW, Australia). The green alga *Chlorella vulgaris* (Beyerinck [Beijerinck]), the diatom *Chaetoceros sp.* and *Isochrysis sp.* (Prymnesiales, Haptophyta) were from the Phuket Marine Biological Centre, Laem Panwa, Phuket 83000. *Synechococcus* and *Chlorella* grew well in BG-11 medium (Allen 1973) and *Chlorella* also grew well in seawater supplemented with nitrate, phosphate and trace elements as for BG-11. No added vitamins were needed. *Chaetoceros*, *Isochrysis* and *Acaryochloris* were grown in seawater supplemented with BG-11 trace elements, 100 mmol m<sup>-3</sup> sodium silicate, 200 mmol m<sup>-3</sup> KH<sub>2</sub>PO<sub>4</sub> and 1 mol m<sup>-3</sup> sodium nitrate. *f/2* vitamins were added as described by McLachlan (1973).

*Synechococcus*, *Acaryochloris*, *Chlorella*, *Chaetoceros* and *Isochrysis* were grown in 250 and 500 mL conical flasks, shaken and stirred daily. Cultures of all four phototrophic microbes were kept on shelves fitted with overhead fluorescent lights (Panasonic 36 W daylight, colour temperature 6500 K: TIS 956-2533) in continuous light at about 27 °C. The light intensity in the culture room was approximately 100-150 μmol photon m<sup>-2</sup> s<sup>-1</sup> (PPFD 400 – 700 nm), measured using a Li-Cor photon flux meter Model LI-189 (Li-Cor Corp, Lincoln, Nebraska, USA).

## Chemicals

DMSO (Dimethylsulphoxide, dimethyl sulfoxide, (CH<sub>3</sub>)<sub>2</sub>SO) was from WINNEX (Thailand) Co. Ltd, Bangkok, Thailand. Acetone (CH<sub>3</sub>)<sub>2</sub>CO 99.5 AR/ACS was from LOBA Chemie PVT. LTD, Mumbai, India. 90% acetone and 100% DMSO were neutralised with magnesium carbonate.

### *Preparation of Cells for Experiments:*

*Synechococcus*, *Acaryochloris*, *Chlorella*, *Chaetoceros* and *Isochrysis* cultures were filtered onto Whatman GF/C glass fibre disks (Whatman International, Maidstone, England, U.K.) using a Millipore apparatus designed for 25 mm filters as described by Ritchie and Runcie (2013). The inside diameter of the Millipore filtration apparatus was 16.2 mm and so the disks of microbial cells adhering to the glass-fibre filter had a surface area of  $206.12 \times 10^{-6} \text{ m}^2$ . The *Synechococcus*, *Acaryochloris*, *Chlorella*, *Chaetoceros* and *Isochrysis*-impregnated disks provided highly reproducible material for experiments. The disks were not allowed to dry out and were placed in a darkened Petri dish with a layer of filter paper moistened with seawater or BG-11 medium as appropriate before making absorbance measurements. Excessive delays in measurements were avoided. Glass fibre filters eventually block if overloaded with cells. Full loading where no more cells could be loaded onto the glass fibre filters varied from one species to another:  $\approx 200 \text{ mg Chl } a \text{ m}^{-2}$  for *Synechococcus*, *Acaryochloris* and *Chlorella* but  $< 100 \text{ mg Chl } a \text{ m}^{-2}$  for *Chaetoceros* and *Isochrysis* because of the mucilaginous nature of the cells.

## ***Scanning Dual Beam Spectrophotometry:***

A standard dual beam scanning spectrophotometer was used for routine chlorophyll determinations (Shimadzu UV-1601, UV-Visible Spectrophotometer, Shimadzu Corporation, Kyoto, Japan, Software: UV-Probe 2.21, Shimadzu Corporation, Kyoto, Japan). Routine chlorophyll determinations were made in  $\text{MgCO}_3$ -neutralised 90% acetone or DMSO (Jeffrey and Humphrey 1975; Ritchie 2006; Ritchie et al. 2021; Ritchie et al. 2022) using quartz cuvettes. *Chlorella* is a recalcitrant alga and heating at  $55 \text{ }^\circ\text{C}$  was usually required to effectively extract chlorophylls. Fewer problems were encountered with the other algae. DMSO is a far better quantitative extractant than acetone. Following our recent practice 850 nm was used as the zero wavelength rather than 750 nm. Routine scans from 850 to 600 nm were used for data acquisition and exported as EXCEL.csv files.

## ***Integrating Sphere Spectrometer:***

A UV Vis Spectrophotometer Model: AE-s90-2D, Serial Number: AT161006, A & E Lab (UK) Co. Ltd fitted with a 60 mm (2 1/2-inch) integrating sphere was used as described in detail in Ritchie and Sma-Air (2020a, b) to measure the optical properties of cell suspensions. The spectrophotometer was run using UV-VIS Analyst version 5.43, prom Version 0.000, Copyright 2013 Macroeasy Technologies Ltd, License number UV 20081012-001-8828-FFF.

## ***Absorbance Measurements using RAT:***

A RGB-diode based leaf absorbance RAT meter was designed by Aquation Pty Ltd, Umina Beach, Australia for the measurement of absorbance of leaves at the same light wavelengths as used by PAM fluorometers (Ritchie and Runcie 2014). The RAT was fitted with a three-colour "RGB" LED as the light source [SML-LX1610RGBW/A diode light source (Lumex Inc., 290 E. Helen Rd, Palatine, IL 60067-6976,

USA)] (Carreres-Prieto et al. 2020). The bandwidths of the RGB diode used in the RAT meter were blue,  $445\pm 15$  nm bandwidth; green,  $525\pm 15$  nm bandwidth and red,  $625\pm 15$  nm bandwidth. Intensities of each colour can be individually adjusted by changing the current to each diode. We have found that the RAT was not only useful for measuring the absorptance properties of leaves and thalli of lichens and macroalgae algae for which it was designed (Ritchie and Runcie 2014) but was also particularly well suited for absorptance readings on algal films mounted upon glass fibre disks (Cebrian et al. 1999; Ritchie 2013; Ritchie and Runcie 2013). The RAT measures transmittance of this light through a specimen to obtain T% and also measures reflectance (R %) using a diode set at  $45^\circ$  to the light beam in an arrangement based upon Schultz (1996) (see Figure 1). Absorptance is calculated as  $Abt\%_{\lambda} = 100 - T\%_{\lambda} - R\%_{\lambda}$  (Runcie and Durako 2004). The meter is calibrated using a black and a white (0 and 100% reflectance respectively) standard card for the particular light source being used (red, green, blue or a RGB combination of sources giving “white” light) following the factory calibration instructions. Some difficulties were encountered in the case of *Acaryochloris* because it absorbs 625 nm light so poorly (Figure 2) for low loadings of the alga on the glass fibre disks, giving zero apparent absorptance for loadings up to about  $30 \text{ mg Chl } d \text{ m}^{-2}$  if the standard white polyester card was used. Satisfactory results on *Acaryochloris* were obtained if a blank glass fibre filter disk was used as a zero rather than the factory supplied white plastic card (see Supplementary Figure). A blank glass fibre disk was also found to be much more satisfactory as a zero for *Isochrysis* than the factory-supplied white card.

Commercial “White Light” diodes are typically configured to have a very high level of blue light and very little green and red light compared to sunlight and so can be misleading for photosynthetic work: in the present study an RGB adjustable for Blue, Green and Red light was used set at blue 50%/green 100%/red 100% to better represent sunlight (Larkum et al. 2018; Carreres-Prieto et al. 2020). Calibration steps involved firstly measuring 100% transmittance with no sample, 0% reflectance with the black card and 100% reflectance with the white standard. The RAT needs to be re-calibrated for each coloured light source.

Saturating absorptance vs. chlorophyll curves were fitted using a simple exponential saturating model. Curves were determined for blue, green and red light and for “white” light. Curves could be determined easily for the algae in the present study with Chl *a* as their primary photosynthetic pigment as previously described for a selection of vascular plants and lichen (Ritchie and Runcie 2014). More caution was needed to make satisfactory measurements of the chlorobacterium, *Acaryochloris marina*, because of the Chl *d + a* pigmentation of the organism (Supplementary Figure).

## ***Statistics:***

Unless otherwise stated all values quoted are means  $\pm$  95% confidence limits with the number of data points quoted in brackets. Using least squares methods and error bars of the fitted parameters  $Abt\%_{\lambda}$ ,  $\infty$  and exponential constant *k* were determined and the asymptotic errors determined by matrix inversion using EXCEL®. Zar (2014) was used as the standard statistical reference text.

## Results

Figure 2 shows *in vivo* integrating sphere scans on *Synechococcus*, *Acaryochloris*, *Chlorella*, *Chaetoceros* and *Isochrysis* standardised onto the blue absorbance peaks for Chl *a* in the cases of *Synechococcus*, *Chlorella* and *Chaetoceros* and *Isochrysis* (436, 434, 439 and 439 nm respectively) and the Chl *d* peak for *Acaryochloris* (455 nm). The *in vivo* scans are based cell suspension with the chlorophyll contents based on 90% acetone extracts ( $\mu\text{g mL}^{-1}$ ,  $n = 4$ ): *Synechococcus*, Chl *a*  $1.534 \pm 0.0927$ ; *Acaryochloris*, Chl *d*  $1.947 \pm 0.198$ , Chl *a*  $0.1089 \pm 0.0125$ ; *Chlorella*, Chl *a*  $2.485 \pm 0.1592$ , Chl *b*  $0.8036 \pm 0.0446$ ; *Chaetoceros* Chl *a*  $4.238 \pm 0.157$ , Chl  $c_1c_2$   $1.146 \pm 0.0367$ ; *Isochrysis*, Chl *a*  $4.02 \pm 0.0317$ , Chl  $c_2$   $1.554 \pm 0.0303$ . *In vivo* pigment peaks: for *Synechococcus* the phycocyanin peak is at 628 nm and the red Chl *a* peak at 677 nm, for *Acaryochloris* the phycocyanin and Chl *a* red peaks were not conspicuous under the conditions under which it was grown, the Chl *d* peak was at 709 nm, for *Chlorella* the Chl *b* “knee” is apparent at about 650 nm and the Chl *a* red peak was at 677 nm, *Chaetoceros* and *Isochrysis* both had Chl  $c_1c_2$  and Chl  $c_2$  peaks at about 630 nm and a Chl *a* peak at 675 nm and a very marked carotenoid peak at 458 nm almost as high as the Chl *a* peak.

The amount of cells that can be loaded onto a glass fibre filter disk is finite because eventually the filter medium becomes clogged if overloaded. The upper cell loading limit for *Synechococcus*, *Acaryochloris* and *Chlorella* was about  $250 \text{ mg Chl } a \text{ m}^{-2}$  for a GFA glass fibre disk (Figs. 3, 4 & 5). The total number of data points was  $n = 26$  (*Synechococcus*) and  $n = 28$  (*Chlorella*). Data were fitted to an exponential saturation curve ( $\text{Abt}\%_{445 \text{ nm}} = \text{Abt}\%_{445 \text{ nm}, \infty} (1 - e^{-k \times \text{Chl } a})$ ) (Chl *d* in the case of *Acaryochloris*) using least squares methods as described by Ritchie and Runcie (2013). Hence, the  $\frac{1}{2}$ -loading point for the cells on a chlorophyll (*a* or *d*) basis was  $\text{Ln}(2)/k$  (Table 1). The exponential saturation model was generally an excellent fit to the experimental data, with significant *r*-values between 0.9574 and 0.9989. In the case of *Synechococcus* (Fig. 3, Table 1) asymptotes were reached in the case of blue, red and “white” light but had not reached asymptotic absorbances in the case of green light even at the maximum practical loading of the alga onto the glass fibre disk ( $\approx 200\text{--}250 \text{ mg Chl } a \text{ m}^{-2}$ ). This is consistent with the poor absorbance of *Synechococcus* in green light ( $\approx 500\text{--}600 \text{ nm}$ ) shown in Fig. 2. For *Synechococcus* the asymptotic  $\text{Abt}\%_{445 \text{ nm}, \infty}$  for disks ( $n = 26$ ) were  $77.3 \pm 0.944$ ;  $\text{Abt}\%_{525 \text{ nm}, \infty} = 74.8 \pm 1.82$ ;  $\text{Abt}\%_{625 \text{ nm}, \infty} = 77.8 \pm 0.950$ ;  $\text{Abt}\%_{\text{white}, \infty} = 75.9 \pm 0.799$ .



Table 1

Fitted parameters Absorbance vs. Chl curves for oxygenic algae. Chl *d* is the primary photosynthetic pigment in *Acaryochloris*, for all the others it is Chl *a*.

Organism	Abt% <sub>λ nm</sub>	Abt% Asymptote at ∞ Chl	Chlorophyll ½-loading point Chl m <sup>-2</sup>	n	r
<i>Synechococcus</i> PCC7942 (Chl <i>a</i> -only)	Abt <sub>445 nm</sub>	77.3 ± 0.944	19.0 ± 1.04	26	0.9978
	Abt <sub>525 nm</sub>	74.8 ± 1.82	363 ± 25.4	26	0.9974
	Abt <sub>625 nm</sub>	77.8 ± 0.950	21.0 ± 1.08	26	0.9981
	“White”	75.9 ± 0.780	24.2 ± 0.975	26	0.9989
<i>Acaryochloris</i> (Chl <i>d</i> )	Abt <sub>445 nm</sub>	79.5 ± 2.18	13.6 ± 1.49	44	0.9737
	Abt <sub>525 nm</sub>	72.2 ± 8.15	49.9 ± 12.6	36	0.9668
	Abt <sub>625 nm</sub>	80.9 ± 4.47	40.3 ± 5.58	14	0.9948
	“White”	73.2 ± 5.02	32.2 ± 6.70	26	0.9663
<i>Chlorella sp.</i> (Chl <i>a + b</i> )	Abt <sub>445 nm</sub>	77.0 ± 2.06	23.0 ± 2.40	28	0.9917
	Abt <sub>525 nm</sub>	87.9 ± 15.7	123 ± 32.8	28	0.9923
	Abt <sub>625 nm</sub>	88.0 ± 16.0	108 ± 30.6	28	0.9917
	“White”	72.1 ± 1.77	54.6 ± 29.7	28	0.9986
<i>Chaetoceros sp.</i> (Chl <i>a + c<sub>1</sub>c<sub>2</sub></i> )	Abt <sub>445 nm</sub>	80.6 ± 1.87	15.5 ± 1.62	28	0.9923
	Abt <sub>525 nm</sub>	81.8 ± 3.14	33.2 ± 3.30	28	0.9961
	Abt <sub>625 nm</sub>	102 ± 16.9	103 ± 21.0	28	0.9952
	“White”	85.1 ± 4.63	35.0 ± 4.72	28	0.9967
<i>Isochrysis sp.</i> (Chl <i>a + c<sub>2</sub></i> )	Abt <sub>445 nm</sub>	83.2 ± 8.06	27.1 ± 9.31	33	0.9574
	Abt <sub>525 nm</sub>	73.1 ± 7.20	34.2 ± 6.49	33	0.9855
	Abt <sub>625 nm</sub>	67.9 ± 5.50	32.5 ± 5.27	33	0.9883
	“White”	62.8 ± 4.27	20.3 ± 3.81	33	0.9713

Figure 4 shows absorbance (Abt%<sub>λ nm</sub>) of *Acaryochloris* cells mounted on GFA Glass fibre disks in blue, green and red light fitted to exponential saturation curves as described for *Synechococcus*. The fitted

parameters are shown in Table 1. *Acaryochloris* absorbs strongly at 445 nm (blue), less strongly at 525 nm (green) and very poorly at 625 nm (red) (Fig. 2). This is because the alga contains predominantly Chl *d* and the red peak of Chl *d* is mainly outside the PPF range and so absorbance in “white” light is hence also rather low (Fig. 2) but the cell suspension absorbs very strongly in the range 350 to 500 nm. The mean  $\text{Abt}\%_{445 \text{ nm}}$  for disks loaded with  $> \approx 100 \text{ mg Chl } d \text{ m}^{-2}$  was  $80.4 \pm 2.94$  (16). More satisfactory results were obtained for *Acaryochloris* at 625 nm if the RGB Rat was zeroed on a blank glass fibre disk (see Supplementary Figure). Whether or not the RAT was zeroed using the factory-supplied white card or blank glass fibre disk did not seem to make a difference for blue, green and “white” light because the alga absorbs strongly in blue and green light (Fig. 2). A range of replication numbers for the different light sources used appears in Table 1 for *Acaryochloris* because a new set of absorptances in red (625 nm) light were needed using a blank glass fibre filter as the white blank rather than the factory supplied white card (see Supplementary Figure).

As in the case of the cyanobacterium, *Synechococcus*, the green alga *Chlorella* has very poor absorbance of light in the range 500 to 600 nm (Fig. 2). Absorptance vs.  $[\text{Chl } a \text{ (mg m}^{-2}\text{)}]$  for *Chlorella* (Fig. 5, Table 1) again followed simple exponential saturation curves but the asymptotic maximum absorptance was not reached within the range of possible loading of the algal cells on the glass fibre disk ( $\approx 100\text{--}250 \text{ mg m}^{-2}$  Chl *a*) for green, red or “white” light but it was in the case of blue light:  $\text{Abt}\%_{445 \text{ nm}, 110\text{--}250 \text{ mg Chl } a} = 76.5 \pm 0.197$  ( $n = 12$ ),  $\text{Abt}\%_{445 \text{ nm}, \infty} = 77.0 \pm 2.06$  ( $n = 28$ ).

For *Chaetoceros*, the upper cell loading limit was about  $122 \text{ mg Chl } a \text{ m}^{-2}$  for a GFA glass fibre disk (Fig. 6, Table 1) and less than  $100 \text{ mg Chl } a \text{ m}^{-2}$  for *Isochrysis* (Table 1, Fig. 7). Absorptance vs.  $[\text{Chl } a \text{ (mg m}^{-2}\text{)}]$  again followed simple exponential saturation curves but the rate at which the asymptotic maximum absorptance was reached was much faster in blue light, slightly slower in the case of green and “white” light and slowest in the case of red light. The  $\text{Abt}\%_{445 \text{ nm}}$  for disks loaded with  $> 60 \text{ mg Chl } a \text{ m}^{-2}$  reached a saturation point for *Chaetoceros* (Fig. 6) and so a maximum standard  $\text{Abt}\%_{445 \text{ nm}, >50 \text{ mg Chl } a}$  of  $78.7 \pm 1.77$  ( $n = 18$ ) could be calculated as a standard absorptance for use with a blue-diode PAM machine for use where discs were loaded with a film of *Chaetoceros* cells with more than  $60 \text{ mg m}^{-2}$  Chl *a*. Blue light reached a saturation point ( $83.2 \pm 8.06$ ,  $n = 33$ ) in the case of *Isochrysis* (Fig. 7) only at near the highest cell loading ( $\approx 100 \text{ mg m}^{-2}$  Chl *a*). In red light (625 nm) the absorptance vs.  $[\text{Chl } a \text{ (mg m}^{-2}\text{)}]$  curve did not even nearly reach an asymptote and so individual absorptances of glass fibre discs impregnated with *Chlorella*, *Chaetoceros* or *Isochrysis* would need to be measured if photosynthesis was to be measured using a red-diode or “white” light PAM mode (Figs. 5, 6 & 7).

## Discussion

The absorbance curves shown in Fig. 2 using an integrating sphere are similar to those already published (Larkum et al. 2018; Ritchie and Sma-Air 2020b) and show that *Synechococcus*, *Acaryochloris*, *Chlorella* and the Chl *c* organisms *Chaetoceros* and *Isochrysis* all strongly absorb blue light due the blue absorption maxima of Chl *a* and *d*. *Acaryochloris* with its unique Chl *d*-based photosynthesis was once

thought to be a very unusual organisms but it is now known to be widespread rather than merely a photosynthetic curiosity (Larkum et al. 2012). Generally blue light absorptance saturates at a lower irradiance than green, red or “white” light (Figs. 3 to 7, Table 1). Saturating absorptances of algal films are often considerably different to the standard default value of  $AbtF\% = 84$  (Björkman and Demmig 1987) and are limited by the loading characteristics of cells onto filter disks.

The colour-temperature of the sun is about 5778 K and so produces relatively little blue light compared to green and red light (Ritchie et al. 2017; Larkum et al. 2018). It is also important that solar energy rapidly attenuates in water with photosynthetically useful red light disappearing in a few meters of water and then green light, such that at depths of greater than about 20 metres only blue light remains (Ritchie et al. 2017; Larkum et al. 2018). In the open ocean, surface inhibition of photosynthesis is well documented but at the depths where photosynthesis is optimum in oceanic water ( $\approx 20$  to 40 m) only blue light is *actually* available for photosynthesis. In aquatic environments the importance of blue light for photosynthesis is perhaps given less attention than it deserves, all the organisms used in this study are very good at absorbing photosynthetically usable blue light in particular diatoms and *Isochrysis* (Figs. 2, 6 & 7, Table 1). Ability to use wavelengths  $> 550$  nm found in the solar spectrum is of more importance to terrestrial and shallow water photosynthesis (Frost-Christensen and Sand-Jensen 1992; Larkum et al. 2018) and *Acaryochloris* can use far red ( $> 690$  nm) for photosynthesis in habitats where blue and 680 nm light is largely filtered out by Chl *a*-based photosynthetic organisms (Larkum et al. 2012).

Figures 3 to 7 show that the RGB-RAT in blue light (445 nm) gives plausible absorptance values ( $Abt\%_{445\text{nm}}$ ) on photosynthetic organisms filtered onto glass fibre disks. The shapes of the absorptance vs. concentration of chlorophyll curves vary considerably from one organism to another but also upon the chosen wavelength. This has important implications on choosing what absorptance data is used for other studies. For example, blue light absorptance data would be appropriate for PAM studies using all five organisms if you were using a blue diode-type PAM machine that used blue light as both the measuring and actinic light source. Red light absorptance data would be appropriate if one wished to measure ETR of the oxygenic photosynthetic organisms with Chl *a* as their primary photosynthetic pigment using a PAM based on red diode technology. The red light (625 nm) of the RGB diode used in the RAT meter may be satisfactory for measuring absorptance of Chl *a* (*Synechococcus*, *Chlorella*, *Chaetoceros* and *Isochrysis*, all with a red-peak at about 676 nm) but not for the red peak absorptance of *Acaryochloris* (709 nm, Chl *d*, Figs. 2 & 4). Absorbance in “white” light and in 630 nm red light is heavily weighted by the phycocyanin present in *Synechococcus* (Figs. 2 & 3). *Chaetoceros* and *Isochrysis* heavily absorb in blue and green light and hence in “white” light (Figs. 2, 6 & 7) but failed to reach asymptotic absorptance in red light (Figs. 6 & 7, Table 1) on the range of disk loadings used in this study. Higher loadings clogged the filter disks. Mucilaginous cells such as many chromophytes (Chl *c*-containing organisms) present difficulties.

The geometry of the RAT meter (Fig. 1) is based on the setup used by Schultz (1996). It uses a light source that unambiguously measures transmittance through the specimen using a photodiode directly under the floor of the measuring chamber. Typically, transmittance near the blue and red *in vivo* peaks for

Chlorophylls is very low (Fig. 2). Reflectance is a more complex issue. The photometer setup used by Schultz (1996) to estimate reflectance has the detector diode set at an angle of 45° to the normal light beam (Fig. 1 in Schultz 1996), essentially the same as the setup used in the RAT meter (Fig. 1) and Fig. 1 in Ritchie and Runcie (2014). This leads to theoretical and experimental problems outlined by Ritchie and Runcie (2014) but an algal or photosynthetic bacterial film on a glass fibre disk is probably closer to a Lambertian surface than a leaf of a vascular plant, in part due to the lack of a reflective waxy cuticle.

The results of experimental measurements of  $Abt_{445\text{ nm}}$  in this study show that the experimentally measured absorptances of glass fibre disks fully loaded with *Synechococcus*, *Acaryochloris*, *Chlorella* or the Chl c-containing *Chaetoceros* and *Isochrysis* have absorptances similar to the default absorptance value ( $Abt\%_F = 84$ ) currently in common use (*Synechococcus*:  $Abt\%_{445\text{ nm}, \infty} = 77.3 \pm 0.94$ ,  $n = 26$ ; *Acaryochloris*:  $Abt\%_{445\text{ nm}, \infty} = 79.5 \pm 2.18$  ( $n = 44$ ); *Chlorella*:  $Abt\%_{445\text{ nm}, \infty} = 77.0 \pm 2.06$  ( $n = 28$ ); *Chaetoceros*  $Abt\%_{445\text{ nm}, \infty} = 80.6 \pm 1.88$  ( $n = 28$ ); *Isochrysis*  $Abt\%_{445\text{ nm}, \infty} = 83.2 \pm 8.06$  ( $n = 33$ ). Thus, the ETR based estimates of photosynthesis of *Chlorella* and *Chaetoceros* made assuming a standard absorptance value of 84% in studies before RAT measurements were available (Ritchie 2008; Ritchie and Runcie 2013; Seatae et al. 2014) were not greatly in error because high enough Chl  $a\text{ m}^{-2}$  loading values were used. This, however, is only fortuitous. In contrast, the standard absorptance value ( $Abt\%_F$ ) of 84 used routinely for vascular plants is a considerable underestimate of absorptance in the case of the leaves of most vascular plants in blue light, where blue-light absorptances typically range from 90 to 95% or higher (Ritchie and Runcie 2014).

The absorptance of a film of unicellular algae or photosynthetic bacteria depends on how many cells are loaded onto the glass fibre disk: this is limited by blockage of the filter. In the case of the experimental organisms used in the present study, the  $Abt\%_{445\text{ nm}}$  vs. concentration of chlorophyll (as  $\text{mg Chl } a\text{ m}^{-2}$ ) follows an exponential saturation curve of the form ( $Abt\%_{445\text{ nm}} = Abt\%_{445\text{ nm}, \infty} \times (1 - e^{-k \times [\text{Chl}]})$ ). The asymptotic absorptance value varies from one organism to another and under different wavelengths of light. In some cases, the asymptotic value is very different to the default  $Abt\%_F$  of 0.84 used as a standard setting in many PAM machines. The kinetic constant ( $k$ ), and hence the  $\frac{1}{2}$  point for saturating loading ( $\text{Ln}(2)/k$ ), varies much more widely than the asymptotic value from one alga to another and in different light regimes.

Figures 3, 4, 5 & 6 show that  $Abt\%_{445\text{ nm}, \text{max}}$  is very close to the asymptotic value ( $Abt\%_{445\text{ nm}, \infty}$ ) if chlorophyll  $a$  loadings are above  $100\text{ mg Chl } a\text{ m}^{-2}$  for *Synechococcus*, *Acaryochloris* and *Chlorella*,  $> 60\text{ mg Chl } a\text{ m}^{-2}$  for *Chaetoceros*. These values for  $Abt_{445\text{ nm}}$  could be used as standard in many circumstances because a Chl  $a$  or Chl  $d$  determination is part of most routine photosynthetic studies and so if the chlorophyll  $a$  or chlorophyll  $d$  loadings onto glass fibre filters exceeded the saturating values for  $\text{Chl } a\text{ m}^{-2}$  the saturating values for absorptance could be used instead of actual absorptance readings. There would be little error in estimates of ETR. In the case of *Isochrysis* it appears to be difficult to reach an optically saturating loading even in blue light (Fig. 7). Absorptances of macroalgae show more variability than one might expect: Figueroa et al. (2009) noted a very troublesome seasonal variability in

*Ulva* which as a flat sheet only two cells thick which one would think presented a very uniform material for photosynthetic studies. Enríquez et al. (2005) showed that there was an exponential saturation curve relationship between chlorophyll *a* content ( $\text{mg m}^{-2}$ ) of seagrass leaves (*Thalassia testudinum*) and absorptance ( $\text{Abt}\%_{400-700 \text{ nm}}$ ). Similar shaped curves were found in Red Maple (*Acer rubrum* L.) (Bauerle et al. 2004). Figures 3 to 7 on unicellular algae loaded onto glass fibre disks show more clearly the relationship between absorptances of photosynthetic surfaces and chlorophyll content than selecting leaves at various stages of development and age and measuring their absorptance and chlorophyll content. These figures help to show that the RGB-RAT gives valid estimates of absorptances.

Asymptotic values for absorptance were found experimentally at the maximum loading of cells in the cases of *Synechococcus* in blue, red and “white” light but not in green light. *Acaryochloris* absorbs strongly in blue and green light and so absorptances as asymptotic or nearly so in blue, green and “white” light (Figs. 2 & 3) but the red light of the RGB diode used in the RAT machine is not suitable for estimating absorptance of a Chl *d*-containing organism at the red absorptance peak for *in vivo* Chl *d* (Figs. 2 & 4). Absorptances of *Chlorella* and the Chl *c*-containing *Chaetoceros* and *Isochrysis* are also strongly asymptotic in blue light. The overall mean asymptote for all the species tested for blue light was  $\text{Abt}\%_{445 \text{ nm}, \infty} \approx 80 \text{ mg Chl } a \text{ m}^{-2}$  and in all species was almost asymptotic in green and “white” light. *Chlorella* and especially *Chaetoceros* and *Isochrysis* did not reach an asymptote in red light: in such cases an asymptotic absorptance cannot be assumed for a high loading of algae onto a glass fibre disk and the absorptance has to be measured experimentally.

Some algae contain photoprotectant compounds similar to anthocyanin found in many vascular plants. Merzlyak et al. (2008) have shown in various tree species that anthocyanin primarily affects absorptance in green and orange light rather than absorptance in blue and red light. Similar conclusions were drawn for *Coleus* varieties heavily pigmented with anthocyanin (Burger and Edwards 1996). Thus anthocyanin does not greatly affect absorptances in blue and red light and so does not cause difficulties in the use of blue or red-diode based PAM machines to estimate ETR in such plants. Anthocyanin does affect the overall absorptance in the PPF range ( $\text{Abt}\%_{400-700 \text{ nm}}$ ) and so the correct absorptance value needs to be estimated when using a PAM with an incandescent light source. Some algae have non-photosynthetic photoprotectant compounds which strongly absorb blue light but not red light and so would affect the amount of photosynthetically useable blue light. The perietin synthesized by the fungal partner in many lichen associations also strongly absorbs blue light (Solhaug et al. 2010). A red-diode based PAM is perhaps the more appropriate PAM to use in such circumstances.

Use of a RGB (Red-Green-Blue) LED diode allows separate measurements of absorptance in “white”, red, green and blue light and is particularly valuable for work with cyanobacteria and rhodophytes which have phycobilin pigments absorbing in the green and orange parts of the spectrum. The disadvantage of using an RGB diode of similar specifications as that used in the present study (SML-LX1610RGBW/A) is that the red wavelength peak is 625–630 nm (a suitable wavelength for human perception of red colour) which is not very close to the *in vivo* red peak of Chl *a* (670–680 nm, Fig. 2) (but is close to the peaks for

Chl  $c_1$  and  $c_2$ ) and is definitely not suitable for measuring at the near-infrared absorbance peak of Chl  $d$  *in vivo* in *Acaryochloris* (Fig. 4). Absorbance values for red, green and blue light also allow an estimation of absorbance in sunlight (5778 K) using methods as described in our previous paper (Ritchie and Runcie 2014) either by the calculation of a mean absorbance from the blue, green and red light absorbances or by adjusting the intensity of the three colour channels to achieve an approximation to “white” light. Some types of PAM machine and other photosynthetic apparatus use red light sources: in such cases the RGB diode source in the RAT device could be replaced by a diode with a more suitable wavelength preferably of the same spectral specification as the light source of the photosynthetic measurement apparatus in question. Unfortunately, the commercially available RGB-diodes are designed for human-eye sensitivity: for photosynthetic purposes a red-diode with a peak at about 670 to 680 nm would be more appropriate.

The RGB RAT Machine described in the present study was designed as a simple portable device suitable for fieldwork (Ritchie and Runcie 2014). Integrating sphere spectrophotometers are now more readily available than previously (Ritchie and Sma-Air 2020b) but require special attachments to measure the transmission ( $T\%_{\lambda}$ ) and reflectance ( $R\%_{\lambda}$ ) and hence absorbance ( $Abt\%_{\lambda}$ ) characteristics of translucent disk material. Using such an integrating sphere setup of a scanning spectrophotometer would allow measurements of absorbance at the red peak of Chl  $d$ -type oxygenic organisms and for photosynthetic bacteria at near infrared wavelengths as well as over their entire photosynthetically active spectrum.

## Abbreviations

$Abt\%_{\lambda \text{ nm}}$  percentage absorbance at wavelength  $\lambda$ ;  $Abt\%_F$ , default Leaf Absorbance Factor as a percentage; CL, confidence limit; E, irradiance ( $\text{mol photon m}^{-2} \text{ s}^{-1}$ ) PPFD; ETR, Absolute Electron Transport Rate; rETR, Relative Electron Transport Rate; PAM fluorometry, Pulse Amplitude Modulation fluorometry; PPFD Photosynthetic Photon Fluence Density (400 – 700 nm);  $P_g$ , Gross Photosynthesis.

## Declarations

### Acknowledgements

We wish to thank Prof A.W.D. Larkum (University of Technology, Sydney, Australia) for his keen interest in the study and helpful input and discussion of the absorbance problem. The Faculty of Environment and Technology of Prince of Songkla University-Phuket provided access to the facilities for the project as part of its policy of promoting the aquaculture industry in Southern Thailand. Andaman Environment and Natural Disaster Research Centre (ANED) also provided facilities and support. Phuket Marine Biological Centre PMBC, Phuket, Thailand) kindly provided the cultures of *Chlorella vulgaris*, *Chaetoceros* and *Isochrysis spp.* *Acaryochloris marina* (MBIC11017) was a gift from Prof Larkum (UTS, Sydney, Australia). The authors declare they have no competing interests in this project.

### Contribution Statement

The two authors Raymond J. Ritchie (RJR) & John W. Runcie (JWR) conceived the project, RJR and Suhailar Sma-Air did most of the experimental work based in Thailand, JWR built the machine and all authors jointly wrote the paper. The authors declare they have no competing interests in this project. All authors have seen and approved of the manuscript.

### Data Availability

The datasets generated during and/or analysed during the current study are available from the corresponding author on reasonable request as EXCEL FILES.

## References

1. Allen MM 1973 Methods for cyanophyceae. In: Stein JR (ed.): Handbook of Phycological Methods: culture methods and growth measurements. Pp. 127–138. Cambridge University Press, Cambridge, U.K.
2. Bauerle WL, Weston DJ, Bowdena JD, Dudley JB, Toler JE 2004 Leaf absorptance of photosynthetically active radiation in relation to chlorophyll meter estimates among woody plant species. *Scientia Horticulturae-Amsterdam* 101:169–178
3. Beach KS, Borgeas HB, Smith CM 2006 Ecophysiological implications of the measurement of transmittance and reflectance of tropical macroalgae. *Phycologia* 45:450–457
4. Beer S, Ilan M, Eschel A, Weil A, Brickner I 1998 Use of pulse amplitude modulated (PAM) fluorometry for in situ measurements of photosynthesis in two Red Sea faviid corals. *Marine Biology* 131:697–612
5. Beer S, Larsson C, Poryan O, Axelsson L 2000 Photosynthetic rates of *Ulva* (Chlorophyta) measured by pulse amplitude modulated (PAM) fluorometry. *European Journal of Phycology* 35:69–74
6. Björkman O, Demmig B 1987 Photon yield of O<sub>2</sub> evolution and chlorophyll fluorescence characteristics at 77K among vascular plants of diverse origins. *Planta* 170:489–504
7. Burger J, Edwards GE 1996 Photosynthetic Efficiency, and Photodamage by UV and Visible Radiation, in Red versus Green Leaf *Coleus* Varieties. *Plant Cell Physiol.* 37:395–399
8. Carr H, Björk M 2003 A methodological comparison of photosynthetic oxygen evolution and estimated electron transport rate in tropical *Ulva* (Chlorophyceae) species under different light and inorganic carbon conditions. *Journal of Phycology* 39:1125–1131
9. Carreres-Prieto D, García JT, Cerdán-Cartagena F, Suardiaz-Muro J 2020 Performing Calibration of Transmittance by Single RGB-LED within the Visible Spectrum. *Sensors* 20:3492, 26p, doi:10.3390/s20123492
10. Cebrian J, Enriquez S, Fortes M, Agawin N, Vermaat JE, Duarte CM 1999 Epiphyte accrual on *Posidonia oceanica* (L.) Delle leaves: implications for leaf absorption. *Botanica Marina* 42:123–128
11. Chandaravithoon P, Nakphet S, Ritchie RJ 2018 Oxygenic and Anoxygenic Photosynthesis in a Sewage Pond. *Journal of Applied Phycology* 30:3089–3102, doi: 10.1007/s10811-018-1423-3


12. Chandaravithoon P, Ritchie RJ, Runcie JW 2020 Measuring Photosynthesis of both Oxygenic and Anoxygenic Photosynthetic Organisms using Pulse Amplitude Modulation (PAM) Fluorometry in Wastewater Ponds. *Journal of Applied Phycology* 32:2615–2629, doi: 10.1007/s10811-020-02171-8
13. Enríquez S, Méndez ER, Iglesias-Prieto R 2005 Multiple scattering on coral skeletons enhances light absorption by symbiotic algae. *Limnology and Oceanography* 50:1025–1032.
14. Figueroa FL, Conde-Álvarez R, Gómez I 2003 Relations between electron transport rates determined by pulse amplitude modulated chlorophyll fluorescence and oxygen evolution in macroalgae under different light conditions. *Photosynthesis Research* 75:259–275
15. Figueroa FL, Martínez B, Israel A, Neori A, Malta E-J, Ang P Jr., Inken S, Marquardt R, Rachamim T, Arazi U, Frenk S, Korbee N 2009 Acclimation of Red Sea macroalgae to solar radiation: photosynthesis and thallus absorptance. *Aquatic Biology* 7:159–172, doi: 10.3354/ab00186
16. Frost-Christensen H, Sand-Jensen K 1992 The Quantum Efficiency of Photosynthesis in Macroalgae and Submerged Angiosperms. *Oecologia* 91:377–384.
17. Genty B, Briantais J-M, Baker, NR 1989 The relationship between the quantum yield of photosynthetic electron transport and quenching of chlorophyll fluorescence. *Biochimica et Biophysica Acta* 990:87–92
18. Hennige SJ, Suggett DJ, Warner ME, McDougall KE, Smith DJ 2009 Photobiology of *Symbiodinium* revisited: bio-physical and bio-optical signatures. *Coral Reefs* 28:179–195
19. Jeffrey SW, Humphrey GF 1975 New spectrophotometric equations for determining chlorophylls a, b, c<sub>1</sub> and c<sub>2</sub> in higher plants, algae and phytoplankton. *Biochemie und Physiologie der Pflanzen (BPP)* 167:191–194
20. Krause, GH, Weis E 1991 Chlorophyll fluorescence and photosynthesis: the basics. – *Annual Review of Plant Physiology* 42:313–349
21. **Larkum AWD, Chen M, Li Y, Schliep M, Trampe E, West J, Salih A, Kühl M (2012) A Novel Epiphytic Chlorophyll  $\alpha$ -containing Cyanobacterium Isolated from a Mangrove-associated Red Alga. *Journal of Phycology* 48:1320-1327**
22. Larkum AWD, Ritchie RJ, Raven JA 2018 REVIEW: Living off the Sun: chlorophylls, bacteriochlorophylls and rhodopsins. *Photosynthetica* 56:11–43, doi: 10.1007/s11099-018-0792
23. Longstaff BJ, Kildea T, Runcie JW, Dennison WC, Hurd C, Kanna T, Raven JA, Larkum AWD 2002 An *in situ* study of photosynthetic oxygen exchange and electron transport rate in the marine macroalga *Ulva lactuca* (Chlorophyta). *Photosynthesis Research* 74:281–293
24. McLachlan J 1973 Growth media – marine. In: Stein JR (ed.): *Handbook of Phycological Methods: culture methods and growth measurements*. Pp. 25–51. Cambridge University Press, Cambridge, U.K.



25. Melis A 1989 Spectroscopic methods in photosynthesis: photosystem stoichiometry and chlorophyll antenna size. *Philosophical Transactions of the Royal Society B* 323:397–409
26. Mercado JM, Jiménez C, Niell FX, Figueroa FL 1996 Comparison of methods for measuring light absorption by algae and their application to the estimation of the package effect. *Scientia Marina* 60:39–45
27. Merzlyak MN, Chivkunova OB, Solovchenko AE, Naqvi KR 2008 Light absorption by anthocyanins in juvenile, stressed, and senescing leaves. *Journal of Experimental Botany* 59:3903–3911
28. Ritchie RJ 2006 Consistent Sets of Spectrophotometric Equations for Acetone, Methanol and Ethanol Solvents. *Photosynthesis Research* 89:27–41.
29. Ritchie RJ 2008 Fitting light saturation curves measured using PAM fluorometry. *Photosynthesis Research* 96:201–215
30. Ritchie RJ 2010 Modelling Photosynthetically Active Radiation and Maximum Potential Gross Photosynthesis. *Photosynthetica* 48:596–609
31. Ritchie RJ 2013 The Use of Solar Radiation by a Photosynthetic Bacterium Living as a Mat or in a Shallow Pond or Flatbed Reactor. *Photochemistry and Photobiology* 89:1143–1162, doi: 10.1111/php.12124
32. Ritchie RJ 2014 Photosynthesis in an Encrusting Lichen (*Dirinaria picta* (Sw.) Schaer.ex Clem., Physciaceae) and Its Symbiont, *Trebouxia* sp, using PAM Fluorometry. *International Journal of Plant Sciences* 175:450–466
33. Ritchie RJ, Heemboom M 2021 *Trentepohlia* sp., a terrestrial chlorophyte growing on galvanised iron lamp posts, *Phycologia* 60:48–61, doi: [10.1080/00318884.2020.1851008](https://doi.org/10.1080/00318884.2020.1851008)
34. Ritchie RJ, Larkum AWD, Ribas A 2017 Could Photosynthesis function on Proxima Centauri b? *International Journal of Astrobiology* 17:147–176, doi: 10.1017/S1473550417000167
35. Ritchie RJ, Runcie JW 2013 Measurement of the Photosynthetic Electron Transport Rate in an Anoxygenic Photosynthetic Bacterium *Afibella* (Rhodospseudomonas) *salina* using PAM Fluorometry. *Photochemistry and Photobiology* 89:370–383
36. Ritchie RJ, Runcie JW 2014 A portable Reflectance-Absorbance-Transmittance (RAT) meter for vascular plant leaves. *Photosynthetica* 52:614–626, doi: 10.1007/s11099-014-0069-y
37. Ritchie RJ, Sma-Air S 2020a Solvent-free chlorophyll spectrometry in unicellular algal research. *Journal of Applied Phycology* 32:2711–2723, doi.org/10.1007/s10811-020-02233-x
38. Ritchie RJ, Sma-Air S 2020b Using integrating sphere spectrophotometry in unicellular algal research. *Journal of Applied Phycology* 32(5):2947–2958, doi.org/10.1007/s10811-020-02232-y
39. Ritchie RJ, Sma-Air S 2022 Photosynthesis of an Endolithic *Chlorococcum* Alga (Chlorophyta, Chlorococcaceae) from Travertine Calcium Carbonate Rocks of a Tropical Limestone Spring. *Applied Phycology* 3:1–15, doi: 10.1080/26388081.2021.2023631
40. Ritchie RJ, Sma-Air S, Dumme V 2022 DMSO formula for chlorophyll determination in dinoflagellates (Chl *a* + *c*<sub>2</sub>). *Journal of Applied Phycology* 34:335–341, doi:10.1007/s10811-021-



41. Ritchie RJ, Sma-Air S, Phongphattarawat S 2021 Using DSMO for Chlorophyll Spectroscopy. *Journal of Applied Phycology* 33:2047–2055, doi: 10.1007/s10811-021-02438-8
42. Rodríguez-Román A, Hernández-Pech X, Thomé PE, Enríquez S, Iglesias-Prieto R 2006 Photosynthesis and Light Utilization in the Caribbean Coral *Montastraea faveolata* Recovering from a Bleaching Event. *Limnology and Oceanography* 51:2702–2710
43. Runcie JW, Durako MJ 2004 Among-shoot variability and leaf-specific absorptance characteristics affect diel estimates of *in situ* electron transport of *Posidonia australis*. *Aquatic Botany* 80:209–220, doi:10.1016/j.aquabot.2004.08.001
44. Schreiber U, Bilger W, Neubaue C 1995 Chlorophyll fluorescence as a non-intrusive indicator for rapid assessment of *in vivo* photosynthesis. In: Schulze, ED, Caldwell, MM (ed.): *Ecophysiology of Photosynthesis: Ecological Studies*, 100. Pp. 49–70. Springer, Berlin.
45. Schultz HR 1996 Leaf absorptance of visible radiation in *Vitis vinifera* L. estimates of age and shade effects with a simple field method. *Scientia Horticulturae-Amsterdam* 66:93–102
46. Seatae P, Bunthawin S, Ritchie RJ 2014 Environmental persistence of chlorine from prawn farm discharge monitored by measuring the light reactions of photosynthesis of phytoplankton. *Aquaculture International* 22:321–338, doi: 10.1007/s10499-013-9642-9.
47. Solhaug KA, Larsson P, Gauslaa Y 2010 Light screening in lichen cortices can be quantified by chlorophyll fluorescence techniques for both reflecting and absorbing pigments. *Planta* 231:1003–1011
48. Stambler N, Dubinsky Z 2005 Corals as light collectors: an integrating sphere approach. *Coral Reefs* 24:1–9
49. Zar JH (2014) *Biostatistical Analysis*. 5<sup>th</sup> edition, Pearson New International Edition Pearson, Edinburgh Gate, Harlow, England, UK. 761 pp.

## Figures



**Figure 1**

Basic arrangement of RGB Light Emitting Diode (RGB-LED) light source and transmittance and reflection detecting photodiodes for measuring absorptance of cells mounted on a filter disc. LEDs are used as the irradiance source. An RGB diode can provide 445 nm (blue), 525 nm (green) or 625 nm (red) light sources. Adapted from Schultz (1996) and Ritchie and Runcie (2014). The working distance is about 2.5 cm.

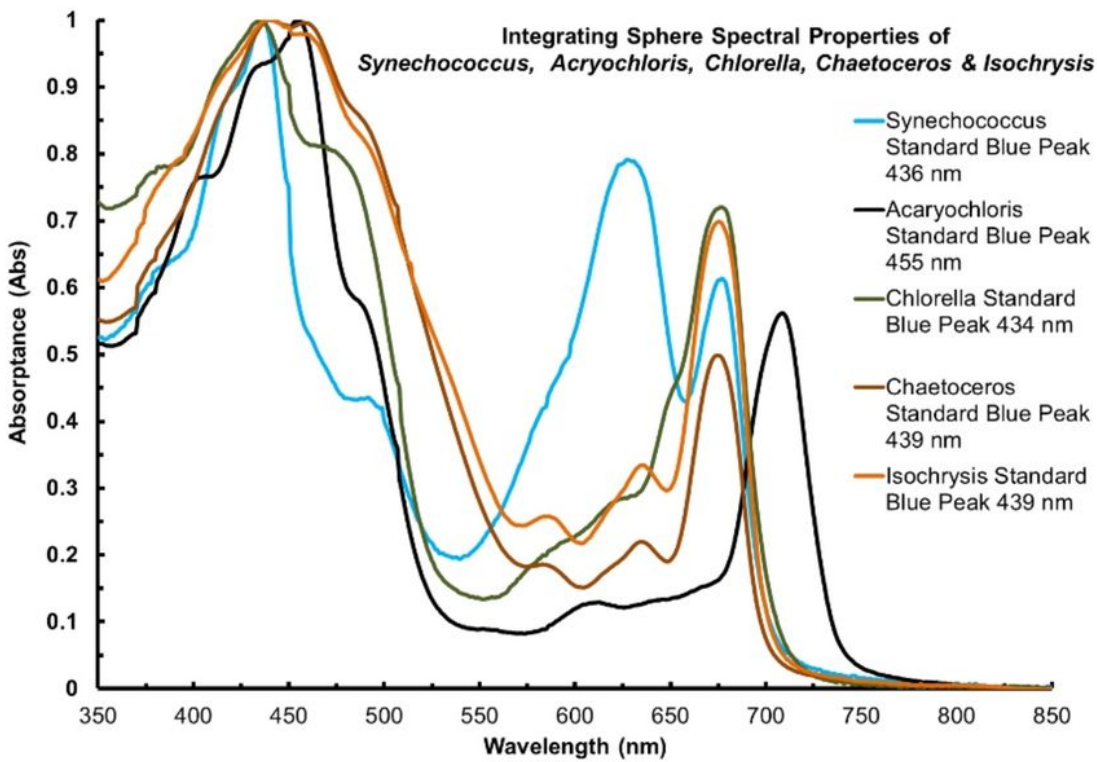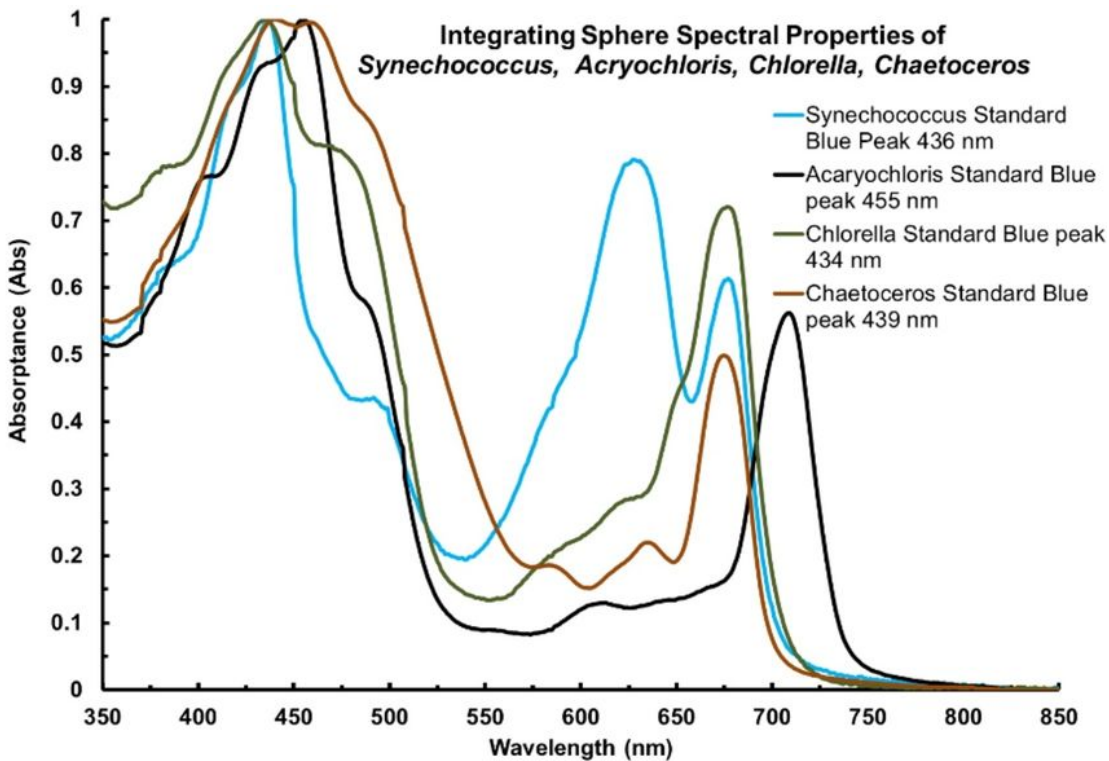

**Figure 2**

Integrating sphere absorbances of cells suspensions of *Synechococcus*, *Acaryochloris*, *Chlorella*, *Chaetoceros* and *Isochrysis* standardised onto the blue absorbance peak after zeroing on 850 nm. The bandwidths of the RGB diode used in the RAT meter were blue,  $445 \pm 15$  nm bandwidth; green,  $525 \pm 15$  nm bandwidth and red,  $625 \pm 15$  nm bandwidth.

### Figure 3

Absorptance ( $\text{Abt}\%_{\lambda \text{ nm}}$ ) of *Synechococcus* cells mounted on GFA Glass fibre disks in blue, green, red and “white” light. Data were fitted to exponential saturation curves ( $\text{Abt}\%_{\lambda \text{ nm}} = \text{Abt}\%_{\lambda \text{ nm}, \infty} (1 - e^{-k \times \text{Chl } a})$ ) using least squares methods for blue (445 nm), green (525 nm) red (625 nm) light and “white” light. The fitted parameters are shown in Table 1. For *Synechococcus* all 4 absorptance curves reached an asymptote within the data range. The mean  $\text{Abt}\%_{445 \text{ nm}}$  for disks loaded with  $> 100 \text{ mg Chl } a \text{ m}^{-2}$  was  $76.8 \pm 1.26$  ( $n = 12$ );  $\text{Abt}\%_{525 \text{ nm}} = 68.71 \pm 2.23$  (12);  $\text{Abt}\%_{625 \text{ nm}} = 76.9 \pm 1.06$  (12), “white”  $\text{Abt}\% = 74.0 \pm 1.43$  (12).

### Figure 4

Absorptance ( $\text{Abt}\%_{\lambda \text{ nm}}$ ) of *Acaryochloris* cells mounted on GFA Glass fibre disks in blue, green and red light fitted to exponential saturation curves as described for *Synechococcus*. The fitted parameters are shown in Table 1. *Acaryochloris* absorbed poorly at 525 and 625 nm and the red peak of Chl *d* is mainly outside the PPF range and so absorbance in “white” light is rather low. The mean  $\text{Abt}\%_{445 \text{ nm}}$  for disks loaded with  $> \approx 100 \text{ mg Chl } d \text{ m}^{-2}$  was  $80.4 \pm 2.94$  (16).

### Figure 5

Absorptance ( $\text{Abt}\%_{\lambda \text{ nm}}$ ) of *Chlorella* cells mounted on GFA Glass fibre disks in blue, green and red light. Data were fitted to exponential saturation curves. The fitted parameters are shown in Table 1. For *Chlorella* only the absorptance vs. Chl *a* curve for blue light reached an asymptote within the experimental range: the mean  $\text{Abt}\%_{445 \text{ nm}}$  for disks loaded with  $> 100 \text{ mg Chl } a \text{ m}^{-2}$  was  $76.5 \pm 1.97$  ( $n = 12$ ) and the asymptotic values was  $\text{Abt}\%_{445 \text{ nm}, \infty} = 77.0 \pm 2.06$  (28) for blue light.

### Figure 6

Absorptance ( $\text{Abt}\%_{\lambda \text{ nm}}$ ) of *Chaetoceros* cells mounted on GFA Glass fibre disks in blue, green, red and “white” light. Data were fitted to exponential saturation curves (Table 1). The green and “white” curves are very similar because of the very high carotenoid content (Figure 2) but the algal disks absorbed very poorly in red light giving an unsatisfactory asymptotic value. For *Chaetoceros* only the absorptance vs. Chl *a* curve for blue light reached an asymptote within the experimental range: the mean  $\text{Abt}\%_{445 \text{ nm}}$  for

disks loaded with 50 to 122 mg Chl  $a$   $m^{-2}$  was  $78.7 \pm 1.77$  ( $n = 18$ ) and the asymptotic value,  $Abt\%_{445 \text{ nm}, \infty} = 80.6 \pm 1.87$  (28).

## Figure 7

Absorptance ( $Abt\%_{\lambda \text{ nm}}$ ) of *Isochrysis* cells mounted on GFA Glass fibre disks in blue, green, red and “white” light. A blank glass fibre disk was used as a blank for all measurements of *Isochrysis*. Data were fitted to exponential saturation curves (Table 1). As in the case for *Acaryochloris* the factory-supplied white card was unsatisfactory for red-diode measurements of *Isochrysis* and so a blank glass fibre disk was used. Within the cell-loading range that could be used (up to  $\approx 100 \text{ mg m}^{-2}$ ) absorptances did not quite reach asymptotes except in the case of blue and “white” light (Table 1).

## Supplementary Files

This is a list of supplementary files associated with this preprint. Click to download.

- [AcaryochlorisRedSupplementary2022.pptx](#)
- [floatimage8.png](#)