



Designation: D892 – 18

British Standard 5092

Designation: 146/2000

Standard Test Method for Foaming Characteristics of Lubricating Oils¹

This standard is issued under the fixed designation D892; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the U.S. Department of Defense.

1. Scope*

1.1 This test method covers the determination of the foaming characteristics of lubricating oils at 24 °C and 93.5 °C. Means of empirically rating the foaming tendency and the stability of the foam are described.

1.2 **WARNING**—Mercury has been designated by many regulatory agencies as a hazardous material that can cause central nervous system, kidney and liver damage. Mercury, or its vapor, may be hazardous to health and corrosive to materials. Caution should be taken when handling mercury and mercury containing products. See the applicable product Material Safety Data Sheet (MSDS) for details and EPA's website—<http://www.epa.gov/mercury/faq.htm>—for additional information. Users should be aware that selling mercury and/or mercury containing products into your state or country may be prohibited by law.

1.3 The values stated in SI units are to be regarded as standard. The values given in parentheses after SI units are provided for information only and are not considered standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.* For specific warning statements, see Sections 7, 8, and 9.1.1.

1.5 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

¹ This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.06 on Analysis of Liquid Fuels and Lubricants.

Current edition approved April 15, 2018. Published May 2018. Originally approved in 1946. Last previous edition approved in 2013 as D892 – 13^{ε1}. DOI:10.1520/D0892-18.

In the IP, this test method is under the jurisdiction of the Standardization Committee. This test method has been approved by the sponsoring committees and accepted by the cooperating societies in accordance with established procedures.

2. Referenced Documents

2.1 ASTM Standards:²

- D445 Test Method for Kinematic Viscosity of Transparent and Opaque Liquids (and Calculation of Dynamic Viscosity)
- D6082 Test Method for High Temperature Foaming Characteristics of Lubricating Oils
- E1 Specification for ASTM Liquid-in-Glass Thermometers
- E128 Test Method for Maximum Pore Diameter and Permeability of Rigid Porous Filters for Laboratory Use
- E1272 Specification for Laboratory Glass Graduated Cylinders

3. Terminology

3.1 Definitions:

3.1.1 *diffuser, n*—for gas, a device for dispersing gas into a fluid.

3.1.1.1 *Discussion*—In this test method the diffuser may be made of either metallic or non-metallic materials.

3.1.2 *entrained air (or gas), n*—in liquids, a two-phase mixture of air (or gas) dispersed in a liquid in which the liquid is the major component on a volumetric basis.

3.1.2.1 *Discussion*—Entrained air (or gas) may form micro size bubbles in liquids that are not uniformly dispersed and that may coalesce to form larger bubbles below or at the surface which break or form foam.

3.1.3 *foam, n*—in liquids, a collection of bubbles formed in or on the surface of a liquid in which the air or gas is the major component on a volumetric basis.

3.1.4 *lubricant, n*—any material interposed between two surfaces that reduces friction or wear between them. **D6082**

3.1.4.1 *Discussion*—In this test method, the lubricant is an oil which may or may not contain additives such as foam inhibitors.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard

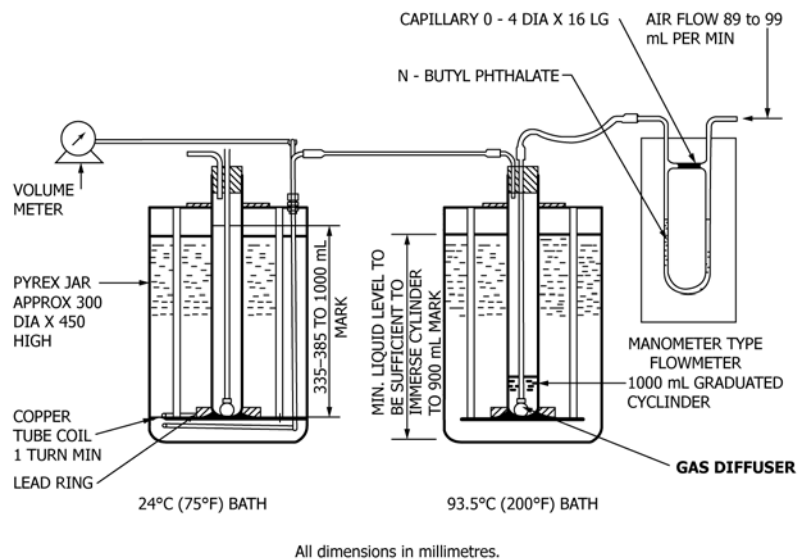


FIG. 1 Foaming Test Apparatus

3.1.5 *maximum pore diameter, n—in gas diffusion*, the diameter of a circular cross-section of a capillary is equivalent to the largest pore of the diffuser under consideration.

3.1.5.1 *Discussion*—The pore dimension is expressed in micrometres (μm).

3.1.6 *permeability, n—in gas diffusion*, the rate of a substance that passes through a material (diffuser) under given conditions.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *dynamic bubble, n*—the first bubble to pass through and escape from the diffuser followed by a continuous succession of bubbles when testing for the maximum pore diameter in Annex A1.

3.2.1.1 *Discussion*—When a diffuser is immersed in a liquid, air can be trapped in the pores. It can escape eventually or as soon as a pressure is applied to the diffuser. When testing for maximum pore diameter (Annex A1) the escape of such bubble shall be ignored.

3.2.2 *foam stability, n*—in foam testing, the amount of foam remaining at the specified time following the disconnecting of the air supply.

3.2.2.1 *Discussion*—In this test method, foam stability is determined from measurements made $10 \text{ min} \pm 10 \text{ s}$ after disconnecting the air supply. In cases after the air supply has been disconnected, where the foam collapses to 0 mL before the 10 min settling time has elapsed, the test may be terminated and the foam stability result recorded as 0 mL.

3.2.3 *foaming tendency, n*—in foam testing, the amount of foam determined from measurements made immediately after the cessation of air flow.

4. Summary of Test Method

4.1 *Sequence I*—A portion of sample, maintained at a bath temperature of $24 \text{ }^\circ\text{C} \pm 0.5 \text{ }^\circ\text{C}$ is blown with air at a constant rate ($94 \text{ mL/min} \pm 5 \text{ mL/min}$) for 5 min, then allowed to settle for 10 min (unless the case described in 3.2.2.1 applies,

in which case, the time duration can be shortened). The volume of foam is measured at the end of both periods.

4.2 *Sequence II*—A second portion of sample, maintained at a bath temperature of $93.5 \text{ }^\circ\text{C} \pm 0.5 \text{ }^\circ\text{C}$, is analyzed using the same air flow rate and blowing and settling time duration as indicated in 4.1.

4.3 *Sequence III*—The sample portion used in conducting Sequence II is used for Sequence III, where any remaining foam is collapsed and the sample portion temperature cooled below $43.5 \text{ }^\circ\text{C}$ by allowing the test cylinder to stand in air at room temperature, before placing the cylinder in the bath maintained at $24 \text{ }^\circ\text{C} \pm 0.5 \text{ }^\circ\text{C}$. The same air flow rate and blowing and settling time duration as indicated in 4.1 is followed.

5. Significance and Use

5.1 The tendency of oils to foam can be a serious problem in systems such as high-speed gearing, high-volume pumping, and splash lubrication. Inadequate lubrication, cavitation, and overflow loss of lubricant can lead to mechanical failure. This test method is used in the evaluation of oils for such operating conditions.

6. Apparatus

6.1 *Foaming Test Apparatus*, an example of a suitable set-up is shown in Fig. 1, consisting of a 1000 mL graduated cylinder or cylinders (meeting Specification E1272 class B tolerance requirement of $\pm 6 \text{ mL}$ and at least graduations of 10 mL) held in position when placed in the baths, such as fitted with a heavy ring or clamp assembly to overcome the buoyancy, and an air-inlet tube, to the bottom of which is fastened a gas diffuser. The gas diffuser can be either a 25.4 mm (1 in.) diameter spherical gas diffuser stone made of fused crystalline alumina grain, or a cylindrical metal diffuser made of sintered five micron porous stainless steel (Note 1). The cylinder shall have a diameter such that the distance from

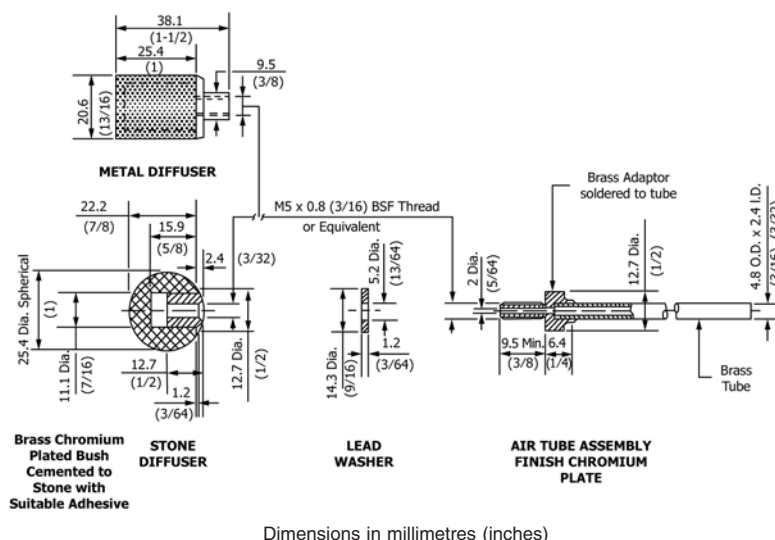


FIG. 2 Attachment of Gas Diffusers to Air-Inlet Tubes

the inside bottom to the 1000 mL graduation mark is 360 mm ± 25 mm. It shall be circular at the top (Note 2) and shall be fitted with a stopper, such as those made of rubber, having one hole at the center for the air-inlet tube and a second hole off-center for an air-outlet tube. The air-inlet tube shall be adjusted so that, when the stopper is fitted tightly into the cylinder, the gas diffuser (Note 3) just touches the bottom of the cylinder and is approximately at the center of the circular cross section. Gas diffusers shall meet the following specification when tested in accordance with the method given in Annex A1:

Maximum pore diameter, μm	Not greater than 80
Permeability at pressure of 2.45 kPa (250 mm) water, mL of air/min	3000 to 6000

NOTE 1—Gas diffuser permeability and porosity can change during use; therefore, it is recommended that diffusers be tested when new and periodically thereafter preferably after each use.

NOTE 2—Graduated cylinders with circular tops can be prepared from cylinders with pouring spouts by cutting them off below the spouts. The cut surface is to be smoothed before use by fire polishing or grinding.

NOTE 3—Gas diffusers may be attached to air-inlet tubes by any suitable means. A convenient arrangement is shown in Fig. 2.

NOTE 4—It may be necessary to confirm the volume of the cylinder.

6.2 *Test Baths*, large enough to permit the immersion of the cylinder at least to the 900 mL mark and capable of being maintained at temperatures constant to 0.5 °C (1 °F) at 24 °C (75 °F) and 93.5 °C (200 °F), respectively. Both bath (Note 6) and bath liquid shall be clear enough to permit observation of the graduations on the cylinder.

NOTE 5—Air baths may also be utilized for heating purposes. Limited data has shown that both liquid and air baths give equivalent results. However, the precision estimates given in Section 13 are based on using only liquid baths.³

NOTE 6—Heat-resistant cylindrical glass jars approximately 300 mm (12 in.) in diameter and 450 mm (18 in.) in height make satisfactory baths.

³ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1516. Contact ASTM Customer Service at service@astm.org.

6.3 *Air Supply*, from a source capable of maintaining an air flow rate of 94 mL/min ± 5 mL/min through the gas diffuser. If the dew point of the air supply does not meet the –60 °C or lower requirements as stated in 7.3, the air shall be passed through a drying tower 300 mm in height packed as follows: just above the constriction place a 20 mm layer of cotton, then a 180 mm layer of indicating desiccant, and a 20 mm layer of cotton. The cotton serves to hold the desiccant in place. Refill the tower when the indicating desiccant begins to show presence of moisture. The use of the drying tower described above is optional if the dew point of the air supply meets the –60 °C or lower requirements as stated in 7.3. A flowmeter sensitive to the required tolerances can be used to measure the air flow (Note 7).

NOTE 7—A manometer type flowmeter, in which the capillary between the two arms of the U-tube is approximately 0.4 mm in diameter and 16 mm in length, and in which *n*-butylphthalate is the manometric liquid, is suitable.

6.3.1 The total volume of air leaving the foaming test apparatus shall be measured by a volume measuring device (Note 9) capable of accurately measuring gas volumes of about 470 mL. The air shall be passed through at least one loop of copper tubing placed around the inside circumference of the cold bath so that the volume measurement is made at approximately 24 °C (75 °F). Precautions are to be taken to avoid leaks at any point in the system.

NOTE 8—Alternatively, a 1 L cylinder (with 10 mL graduation marks) full of water is inverted in a tall, large beaker also filled with water. There should be no air bubbles inside. Air leaving the copper loop in the bath is connected below the cylinder. When the test is started, air will flow into the cylinder, displacing the water. At the end of the test, the volume of air in the cylinder is measured by equalizing the water levels inside and outside the cylinder. Alternatively, the total volume of air passed would be the difference between the final and the initial volumes of water in the cylinder.

NOTE 9—A wet test meter calibrated in hundredths of a litre is suitable.

6.4 *Timer*; graduated and accurate to 1 s or better.

6.5 *Temperature Sensing Device*, capable of covering the temperature range from at least 20 °C to 100 °C, with an accuracy of ± 0.5 °C. A thermometer having a range as shown below and conforming to the requirements as prescribed in Specification E1 or specifications for IP thermometers has been found suitable to use:

Temperature Range	Thermometer	No. IP
20 °C to 102 °C	ASTM 12C	64C

7. Reagents and Materials

7.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all cases. Unless indicated otherwise, it is intended that all reagents conform to the specifications of the committee on Analytical Reagents of the American Chemical Society where such specifications are available.⁴ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

7.2 *Acetone*—(**Warning**—Extremely flammable, vapors can cause a flash fire).

7.3 *Compressed Air*, hydrocarbon free and dry to a dew point of -60 °C or lower, otherwise the drying tower described in 6.3 shall be used.

7.4 *Cleaning Reagents*—such as heptane (**Warning**—Flammable, vapor harmful) and toluene (methylbenzene) for use in cleaning the cylinder, gas diffuser, and air-inlet tube. Other reagents with equivalent cleaning and solvency characteristics may be substituted as appropriate, provided the requirements in 9.1 are satisfied.

7.5 *Propan-2-ol*—for use in determining the maximum pore diameter if a metallic diffuser is used (see A1.2.1). (Solvents with equivalent cleaning and solvency characteristics may be substituted for propan-2-ol.)

8. Hazards

8.1 (**Warning**—Users of this test method shall be trained and familiar with all normal laboratory practices, or under the immediate supervision of such a person. It is the responsibility of the operator to ensure that all local legislative and statutory requirements are met.)

8.2 (**Warning**—Cleaning solvents have flash points lower than ambient temperatures. Avoid the possibility of fire or explosion.)

8.3 (**Warning**—The fumes from the test oil and the bath shall be vented in a manner compatible with local government regulations.)

8.4 (**Warning**—Some apparatus assemblies can have as much as 20 L of heat transfer oil at 93.5 °C. Therefore, in the

event of breakage of the containing vessel, provisions for suitable containment of the spill is advisable.)

9. Preparation of Apparatus

9.1 Thorough cleansing of the test cylinder (9.1.1) and gas diffuser and air-inlet tube (9.1.2) is essential after each use to remove any additive remaining from previous tests which can seriously interfere with results of subsequent tests. The criterion that the test cylinder is adequately cleaned is that the interior walls drain water cleanly, without drops forming. As for the gas diffuser and air-inlet tube, the criterion for adequate cleaning is that no visual evidence of residual material remains from a prior analysis prior to conducting a subsequent analysis.

9.1.1 *Cylinder*—One suitable technique for cleaning the cylinder is to rinse the cylinder with heptane. (**Warning**—Flammable, vapor harmful.) Wash the cylinder with a suitable detergent. Rinse the cylinder, in turn, with distilled water, then acetone (**Warning**—Extremely flammable, vapors can cause a flash fire) and dry in a current of the compressed air or in a drying oven.

NOTE 10—Certain detergents are notorious for adhering to glass; therefore, it is important to realize that such a circumstance can affect the test result. Several rinsings with water and acetone may be required.

9.1.2 *Gas Diffuser and Air Tube*—One suitable technique for cleaning the gas diffuser and air tube is to first clean the inside of the air tube (disassembled from the gas diffuser) with toluene and heptane. Next, connect the air tube and gas diffuser and immerse the gas diffuser in about 300 mL of toluene. Flush a portion of the toluene back and forth through the gas diffuser at least five times with vacuum and air pressure. Repeat the process with heptane. After the final washing, dry both the air tube and the gas diffuser thoroughly by forcing clean air through them (see Note 11). Wipe the outside of the air inlet tube, first with a cloth moistened with heptane, then a dry cloth. Do not wipe the gas diffuser.

NOTE 11—Certain samples may contain ingredients which may not be adequately removed by this process and, because these can affect the next test, more rigorous cleaning may be required; this is recommended. When alternate diffuser cleaning methods are used certain cautions should be observed: (1) Non-metallic diffusers may have adsorbed as well as adsorbed these interfering ingredients or the cleaners, or both, and this shall be considered before proceeding to the next test. (2) So that all tests performed start off under the same circumstances, when alternate diffuser cleaning methods are used, the final rinsing process shall be as detailed in 9.1.2. (3) See also Note 1.

10. Procedure

10.1 *Sequence I*—Without mechanical shaking or stirring, decant approximately 200 mL of sample into a beaker (see 10.1.1). Heat to 49 °C \pm 3 °C and allow to cool to 24 °C \pm 3 °C. See Option A for stored sample (see 10.5). Each step of the procedure described in 10.3 and 10.4, respectively, shall be carried out within 3 h after completion of the previous step. In 10.5.1, the test shall be carried out as soon as compatible with the temperature specification and not more than 3 h after immersion of the cylinder in the 93.5 °C (200 °F) bath.

10.1.1 If a sample arrives in the lab and it has been determined that it is at or above 49 °C \pm 3 °C, the heating step in 10.1 may be eliminated. Heating the sample to 49 °C \pm 3 °C

⁴ *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For Suggestions on the testing of reagents not listed by the American Chemical Society, see *Annual Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

in 10.1 is intended to remove any thermal history before proceeding, which is not an issue for samples arriving in the lab already at or above $49\text{ °C} \pm 3\text{ °C}$.

10.2 Pour the sample into the 1000 mL cylinder until the liquid level is at the 190 mL mark. Visually estimate the level to be within 5 mL. Immerse the cylinder at least to the 900 mL mark in the bath maintained at $24\text{ °C} \pm 0.5\text{ °C}$ ($75\text{ °F} \pm 1\text{ °F}$). When the oil has reached the bath temperature, insert the gas diffuser and the air-inlet tube with the air source disconnected, and permit the gas diffuser to soak for about 5 min. Connect the air-outlet tube to the air volume measuring device. At the end of 5 min, connect to the air source, adjust the air flow rate to $94\text{ mL/min} \pm 5\text{ mL/min}$, and force clean dry air through the gas diffuser for $5\text{ min} \pm 3\text{ s}$, timed from the first appearance of air bubbles rising from the gas diffuser. At the end of this period, shut off the air flow by disconnecting the hose from the flow meter and immediately record the volume of foam; that is, the volume between the oil level and the top of the foam. The total air volume which has passed through the system shall be $470\text{ mL} \pm 25\text{ mL}$. Allow the cylinder to stand for $10\text{ min} \pm 10\text{ s}$ and again record the volume of foam (see 10.2.1).

10.2.1 In cases after the air supply has been disconnected, where the foam collapses to 0 mL before the 10 min settling time has elapsed, the test may be terminated and the foam stability result recorded as 0 mL.

10.3 *Sequence II*—Pour a second portion of sample into a cleaned 1000 mL cylinder until the liquid level is at the 180 mL mark. Visually estimate the level to be within 5 mL. Immerse the cylinder at least to the 900 mL mark in the bath maintained at $93.5\text{ °C} \pm 0.5\text{ °C}$. When the oil has reached and equilibrated with the bath temperature requirements in 10.2 (see 10.3.1), insert a clean gas diffuser and air-inlet tube and proceed as described in 10.2, recording the volume of foam at the end of the blowing and settling periods. In cases where 10.2.1 applies, the test procedure may continue to Sequence III.

10.3.1 One way to verify the oil temperature has equilibrated with the bath temperature is by checking the oil temperature directly and ensuring the temperature is within the limits indicated in 10.3 before proceeding. This practice of checking the oil temperature until the value is within required limits before proceeding has led some laboratories to determine the minimum soak time necessary (based on their specific bath design and corresponding temperature-monitoring study results) for any oil sample to reach bath temperature equilibrium. This information has been used to apply this minimum soak time to subsequent samples without the need to verify the oil temperature before proceeding. In cases where a laboratory chooses to set minimum soak time requirements, the onus is on the laboratory to maintain the necessary temperature-monitoring study information as appropriate.

10.4 *Sequence III*—Collapse any foam remaining after the test at 93.5 °C (200 °F) (10.3), by stirring. Cool the sample to a temperature below 43.5 °C (110 °F) by allowing the test

cylinder to stand in air at room temperature, then place the cylinder in the bath maintained at $24\text{ °C} \pm 0.5\text{ °C}$ ($75\text{ °F} \pm 1\text{ °F}$). After the oil has reached bath temperature, insert a cleaned air-inlet tube and gas diffuser and proceed as described in 10.2, recording the foam value at the end of the blowing and settling periods. (See 10.2.1.)

10.5 Some lubricants with modern additives can pass their foam requirements when blended (with the antifoam properly dispersed in small particle sizes) but fail to meet the same requirements after two or more weeks' storage. (It appears that the polar dispersant additives have the potency to attract and hold antifoam particles, such that the apparent increased antifoam size results in decreased effectiveness to control foam in Test Method D892.) However, if the same stored oil is merely decanted and poured into engines, transmissions, or gear boxes and those units operated for a few minutes, the oil again meets its foam targets. Similarly, *decanting* the stored oil into a blender, followed by agitation as described for Option A (see 10.5.1), redisperses the antifoam held in suspension and the oil again will give good foam control in Test Method D892. For such oils, Option A can be used. On the other hand, if the antifoam is not dispersed into sufficiently small particles when the oil is blended, the oil cannot meet its foam requirements. If this freshly blended oil were vigorously stirred according to Option A, it is very possible that the oil would then meet its foam targets whereas the plant blend would never do so. Therefore, it is inappropriate and misleading to apply Option A for quality control of freshly made blends.

10.5.1 *Option A*—Clean the container of a 1 L (1 qt), high-speed blender using the procedure given in 9.1.1. Place 500 mL of sample measured from 18 °C to 32 °C (65 °F to 90 °F) into the container, cover, and stir at maximum speed for 1 min. Because it is normal for considerable air to be entrained during this agitation, allow to stand until entrained bubbles have dispersed and the temperature of the oil has reached $24\text{ °C} \pm 3\text{ °C}$ ($75\text{ °F} \pm 5\text{ °F}$). Within 3 h following the agitation (solvents with equivalent cleaning and solvency characteristics may be substituted for toluene), start with testing as specified in 10.2.

NOTE 12—In case of viscous oils, 3 h can be insufficient time to disperse the entrained air. If a longer time is required, record the time as a note on the results.

11. Alternative Procedure

11.1 For routine testing a simplified testing procedure can be used. This procedure differs from the standard method in only one respect. The total air volume used during the 5 min blowing period is not measured after the air has passed through the gas diffuser. This eliminates the volume measuring equipment and the airtight connections necessary to carry the exit air from the graduated cylinder to the volume measuring device, but requires that the flowmeter be correctly calibrated and that the flow rate be carefully controlled. Results obtained by this procedure shall be reported as D892 – IP 146 (Alternative).

12. Report

12.1 Report the data in the following manner:

Test	Foaming Tendency ASTM	Foam Stability ASTM
	D892 IP 146	D892 IP 146
	Foam Volume, mL, at end of 5 min blowing period	Foam Volume, mL, at end of 10 min settling period
<i>As received:</i>		
Sequence I
Sequence II
Sequence III
<i>After agitation:</i>		
<i>(Option A, 10.5.1)</i>		
Sequence I
Sequence II
Sequence III

12.2 For the purpose of reporting results, when the bubble layer fails to completely cover the oil surface and a patch or eye of clear fluid is visible, the value shall be reported as nil foam.

13. Precision and Bias⁵

13.1 Precision—The precision values in this statement were determined in a cooperative laboratory program.⁶

13.1.1 Repeatability—The difference between successive results obtained by the same operator with the same apparatus under constant operating conditions on identical test material would, in the long run, in the normal and correct operation of the test method exceed the following values in only one case in twenty.

⁵ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1244. Contact ASTM Customer Service at service@astm.org.

⁶ Filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1007. Contact ASTM Customer Service at service@astm.org.

Seq. I Tendency:
Repeatability = 0.7076X^{0.7909}

Seq. II Tendency:
Repeatability = 0.2119(X + 27.1933)

D892, Seq. III Tendency:
Repeatability = 1.3640X^{0.6872}

NOTE 13—For Sequence I precision, there is no data in the region 100 mL to 500 mL due to rejection of the two samples in that region.

13.1.2 Reproducibility—The difference between two single and independent results obtained by different operators working in different laboratories on identical test material would, in the long run, exceed the following values in only one case in twenty.

Seq. I Tendency:
Reproducibility = 1.1195X^{0.7909}

Seq. II Tendency:
Reproducibility = 0.4408(X + 27.1933)

D892, Seq. III Tendency:
Reproducibility = 2.6996X^{0.6872}

13.1.3 For those oils which have been tested by Option A (10.5.1), no precision statement is yet available.

NOTE 14—The majority of the results in the cooperative work that led to Option A were nil foam; hence, no precision statement can be calculated.

13.2 Bias—Since there is no accepted reference material suitable for determining the bias for the procedure for measuring foaming characteristics in Test Method D892, bias cannot be determined.

14. Keywords

14.1 foam (foaming)

ANNEX

(Mandatory Information)

A1. TEST FOR MAXIMUM PORE DIAMETER AND PERMEABILITY OF GAS DIFFUSERS (BASED ON TEST METHOD E128)

A1.1 Apparatus

A1.1.1 One example of a suitable apparatus that can be used for the maximum pore diameter determination consists of a regulated source of clean, dry, compressed air, a U-tube water manometer of sufficient length to read a pressure differential of 7.85 kPa (800 mm of water) and a cylinder of a size sufficient (250 mL is suitable) to conveniently immerse a gas diffuser to a depth of 100 mm (see Fig. A1.1). Other apparatus and set-ups capable of accurately determining the maximum pore diameter of the gas diffusers by regulating the air flow by alternate means to provide the required pressure differential can also be used. In such cases, it is permissible to make the necessary updates to the procedure in A1.2.1 and A1.2.1.1 as appropriate.

A1.1.2 One example of additional apparatus found suitable for determining permeability consists of a gas volume metre of

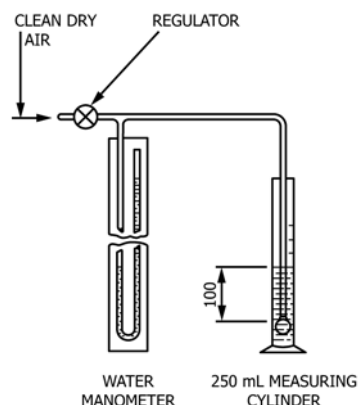


FIG. A1.1 Apparatus for Measuring Maximum Pore Size

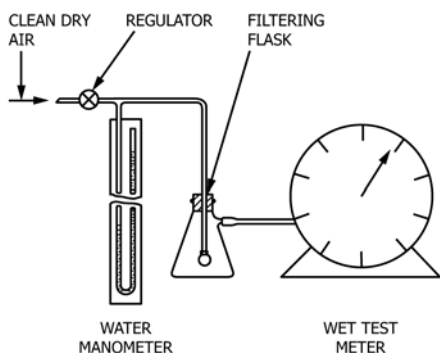


FIG. A1.2 Apparatus for Measuring Permeability

sufficient capacity to measure flow rates of at least 6000 mL/min while generating a back pressure of no more than 10 mm water. A filtering flask large enough that the 25.4 mm (1 in.) diameter diffuser will pass through the neck. This flask shall be fitted with a rubber stopper with a single hole to admit the air-inlet tube (see Fig. A1.2). A supply of tubing having an internal diameter of 8 mm (0.3 in.) shall be used to make the connections between the various parts of the apparatus as shown in Fig. A1.1 and Fig. A1.2. Other apparatus and set-ups capable of accurately determining the permeability of the gas diffusers by regulating the air flow by alternate means to provide the required pressure differential can also be used. In such cases, it is permissible to make the necessary updates to the procedure in A1.2.2 as appropriate.

A1.2 Procedure

A1.2.1 *Maximum Pore Diameter*—Connect the diffuser to the manometer using an adaptor as shown in Fig. 2 (but without the brass tubing) and a 1.0 m length of 8 mm bore tubing. Support the clean diffuser to a depth of 100 mm, as measured to the top of the diffuser, in distilled water if the diffuser is non-metallic and propan-2-ol if the diffuser is metallic. Allow to soak for at least 2 min. Connect the air-inlet tube to a controllable source of clean, compressed air as shown in Fig. A1.1. Increase the air pressure at a rate of about 490 Pa (50 mm of water)/min until the first dynamic bubble passes

through the filter and rises through the water. The first dynamic bubble is recognized by being followed by a succession of additional bubbles. Read the water level in both legs of the manometer and record the difference p . The uniformity of distribution of pores approaching maximum pore size may be observed by gradually increasing the air pressure and noting the uniformity with which streams of bubbles are distributed over the surface.

A1.2.1.1 Calculate the maximum pore diameter, D , in micrometres, as follows:

(1) For non-metallic diffusers and water as the diffuser medium:

$$D = 29\,225/(p - 100) \quad (A1.1)$$

where:

p = mm of water.

(2) For metallic diffusers and propan-2-ol as the diffuser medium:

$$D = 8930/(p - 80) \quad (A1.2)$$

where:

p = water in the manometer, mm.

A1.2.1.2 Calibration of diffusers have been found to be a critical factor in this test.⁷

A1.2.2 *Permeability*—Connect the clean, dry diffuser with a controllable source of clean, dry, compressed air, again using a 1 m length of 8 mm-bore tubing, and place it in a filtering flask connected to a suitable flowmeter using a further 0.5 m length of tubing as shown in Fig. A1.2. Adjust the pressure differential to 2.45 kPa (250 mm of water) and measure the rate of flow of air through the gas diffuser in millilitres per minute. Depending on the sensitivity of the flowmeter used, this observation may be made for a suitably longer period and the average flow rate per minute recorded.

⁷ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1369. Contact ASTM Customer Service at service@astm.org.

APPENDIXES

(Nonmandatory Information)

X1. HELPFUL HINTS FOR OPERATION OF TEST METHOD D892

X1.1 Helpful Hints

X1.1.1 The test should be performed exactly as described to obtain good results.

X1.1.2 Norton stone diffusers are known to be unreliable regarding their porosity and permeability; hence, new stones (as well as the metal diffusers) need to be checked in accordance with Annex A1.

X1.1.3 The diffusers should be checked periodically for porosity and permeability, depending upon the usage; checking is recommended at least once a week. Out of specification diffusers are a major cause of inaccuracy in this test method.

X1.1.4 The connection between the gas diffusers and the air inlet tubes should be airtight.

X1.1.5 The inlet air should be dried by passing through a desiccant drying tower. The indicator desiccant needs to be changed when it shows the presence of moisture by changing its color from blue to pink.

X1.1.6 If a thermometer is used as the temperature sensing device (see 6.5), thermometer calibration should be checked at least annually against a master thermometer. For other temperature sensing devices, checking the calibration at least annually against a traceable source is also recommended.

X1.1.7 Thorough cleaning of the test cylinder and the air inlet tube is essential after each use to remove any residual additive from the previous analysis.

X1.1.7.1 The cylinders are cleaned with heptane, a suitable detergent, distilled water, acetone, and dried with air or in an oven, in sequence.

X1.1.7.2 The gas diffusers are cleaned at least five times with toluene, heptane, and clean dry air in sequence.

X1.1.8 Oil or water baths must be used to control testing temperatures within 0.5 °C (1 °F).

X1.1.9 The total volume of the air passing through the system should be measured to 470 mL ± 25 mL. Without this step, there is no way of ascertaining that the system is airtight.

X1.1.10 It is recommended that the stopwatches be calibrated against a national standard at least once a year. Annex A3 (Timer Accuracy) of Test Method D445 is a good source for guidance on how to check the timers for accuracy.

X1.1.11 If using Option A, all entrained air bubbles after stirring should be dispersed before testing.

X1.1.12 It is misleading and inappropriate to apply Option A for quality control of freshly made blends, or comparing/reporting Option A and regular foam test results.

X1.1.13 If the alternative procedure is used for measurements, the data should not be reported as that obtained by Test Method D892.

X1.1.14 In 6.1, verify the distance between inside bottom of the cylinder and the 1000 mL graduation mark.

X1.1.15 In 6.1, a diffuser centering washer is used to ensure the diffuser head is centered within the cylinder to eliminate wall interference with foam generation and expansion during and after the blowing period. This is particularly helpful when dark fluids are tested or lighting conditions or darkened bath liquids make centering difficult.

X1.1.16 In 6.1, hold the cylinders in an upright position by use of a suitable device. If the cylinders are not vertical or move during the test, or both, foam level errors can be increased.

X1.1.17 In 9.1.2, avoid touching the diffusers with one's hands.

X1.1.18 In 10.2 – 10.4, verify that the sample has reached the bath temperature before starting the measurements.

X2. 2003 INTERLABORATORY STUDY PRECISION TECHNIQUE

X2.1 An Interlaboratory Study (ILS) was organized to improve precision of Test Method D892. Twelve laboratories participated in the ILS.

X2.1.1 Participating laboratories included ten user laboratories, one commercial test laboratory, and one foam test instrument manufacturer's laboratory. Eight of the laboratories used liquid baths and four used air baths. All laboratories used only new and calibrated metal diffusers, and all laboratories were equipped with the same type of device for measuring the air actually passing through the diffuser and fluid as schematically shown in Fig. X2.1.

NOTE X2.1—Any device for precisely measuring the actual volume required for the test can be used.

X2.1.2 Five samples consisting of three engine oil types, a base oil, and a commercially available reference oil were analyzed in duplicate.

X2.2 Some deviations from Test Method D892 were specified. The main deviations included:

X2.2.1 Samples were upended 20 times before being put into the test cylinder.

NOTE X2.2—This differs from 10.1 of the test method in specifying effective and precisely repeatable mixing of the sample rather than the highly variable and vigorous mixing specified in Option A.

X2.2.2 A diffuser centering washer was used to ensure the diffuser head was accurately centered within the glass cylinder during the 5-min blowing period. This is shown in Fig. X2.2.

X2.2.3 There was no more than a 1 h delay after heating. 10.1 allows up to a 3 h delay.

X2.2.4 An effective commercial glass cleaning agent was specified in addition to the cylinder cleaning steps in 9.1.1 of the test method to ensure cylinders were thoroughly cleaned of oil residue prior to each test run.

X2.2.5 The procedure for Option A for blending was not used.

X2.2.6 The alternative procedure (11.1 of the test method) was not used. Instead, it is required to measure the air passing through the diffuser and test fluid with an exit air volume measuring device.

NOTE X2.3—For operators looking to improve consistency and test precision, the remaining sections of Appendix X2 offer further clarification of techniques from the ILS not presently in Test Method D892. Complete details of the ILS are described in an ASTM Research Report being prepared to be submitted to ASTM International Headquarters.

X2.3 *Diffuser Centering Washer*—Thin washer (1 mm thick) whose overall diameter is slightly smaller than the cylinder diameter and whose center diameter is 4 mm larger than the diameter of the diffuser.

X2.4 *Commercial Glass Cleaning Agent*—capable of removing oil residue and varnish from glassware.

X2.4.1 After cleaning the cylinder according to 9.1.1, wash the cylinder interior with commercial cleaning agent. Rinse with warm water and allow to thoroughly dry.

NOTE X2.4—For more effective cleaning, periodically fill the cylinder with commercial cleaning agent and allow to soak for 30 m. Rinse with warm water and allow to dry.

X2.5 *Sequence I* (see 10.1)—Slowly invert the container of test fluid 180° and return to upright 20 times (2 s minimum for each inversion cycle) by hand (or rotate by machine). Do not shake container. Follow the remainder of 10.1 – 10.4. However, Option A (10.5) shall not be used.

X2.6 Do not use the alternative procedure shown in 11.1.

NOTE X2.5—Alternative procedures, which depend on measuring rate of incoming air (gas) flow rather than the total volume of air (gas) flow that has passed through the diffuser, have been found questionable as a result of undetected leakage of the tubing connecting the air (gas) to the diffuser or undetected changes in the porosity of the diffusers.

X2.7 The following precision and bias statements were obtained from this ILS:⁸

X2.7.1 *Repeatability*—The difference between successive results obtained by the same operator with the same apparatus under constant operating conditions on identical test material would, in the long run, in the normal and correct operation of the test method, exceed the values shown below and in Fig. X2.3 in only 1 case in 20.

Sequence	Repeatability
I	0.10 (x + 55)
II	0.10 (x + 44)
III	0.15x

where x = the determined value.

X2.7.2 *Reproducibility*—The difference between successive results obtained by different operators with different apparatuses in different laboratories on identical test material would, in the long run, in the normal and correct operation of the test method, exceed the values shown in below and in Fig. X2.4 in only 1 case in 20.

Sequence	Reproducibility
I	0.29 (x + 55)
II	0.26 (x + 44)
III	0.44x

where x = the determined value.

X2.7.3 *Bias*—Since there is no accepted reference material suitable for determining the bias for the procedure for measuring foaming characteristics in Appendix X2 of Test Method

D892, bias cannot be determined.

Sketch of Foam Bath Set-Up Using Exit Air Volume Measurement

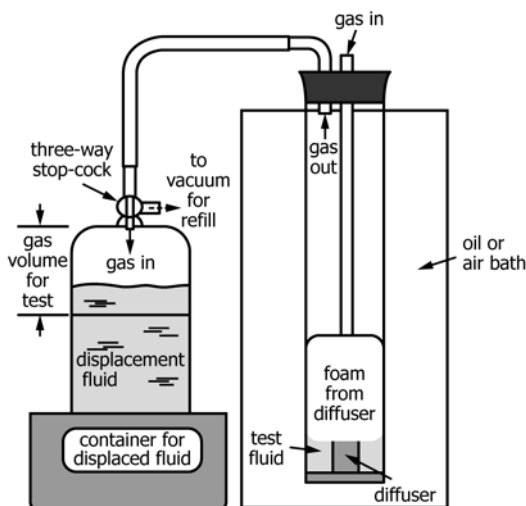


FIG. X2.1 Set-up of Exit Air Measurement

Cut-away Sketch of Cylinder Set-Up

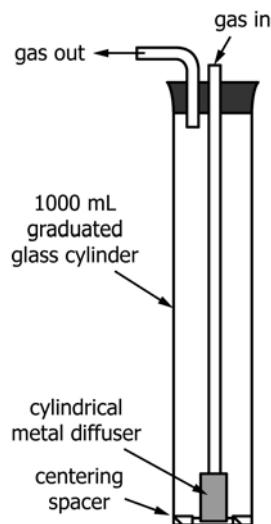


FIG. X2.2 Set-up of Graduated Cylinder with Spacer

⁸ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1618. Contact ASTM Customer Service at service@astm.org.

Foam Tendency Repeatability - Sequences I, II, and III

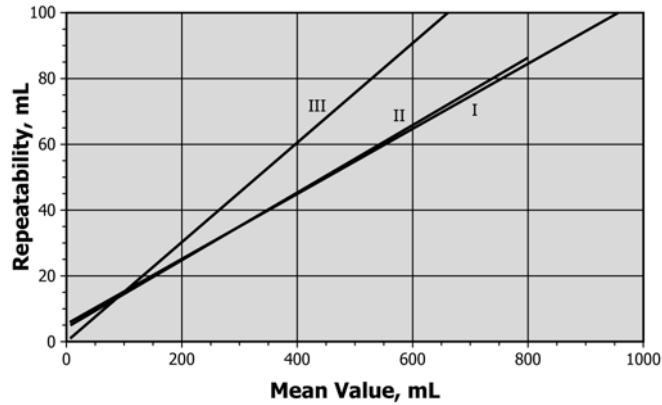


FIG. X2.3 Repeatability of Foam Tendency for All Three Sequences

Foam Tendency Reproducibility - Sequences I, II, and III

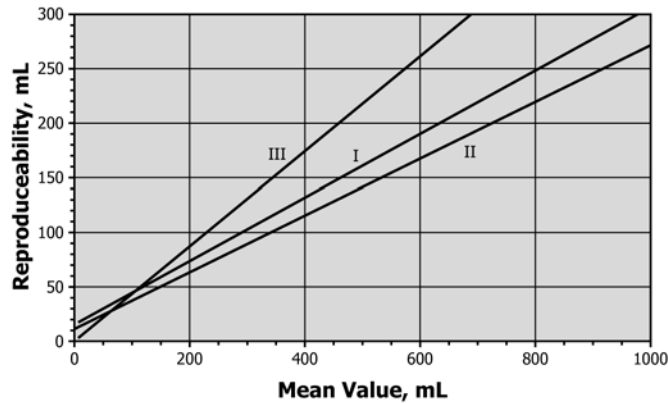


FIG. X2.4 Reproducibility of Foam Tendency for All Three Sequences

SUMMARY OF CHANGES

Subcommittee D02.06 has identified the location of selected changes to this standard since the last issue (D892 – 13^{e1}) that may impact the use of this standard. (Approved April 15, 2018.)

- (1) Revised subsections 13.1.1 and 13.1.2, removing former Figures 3 and 4.
- (2) Deleted former Note 13.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/